

TECHNICAL SPECIFICATION

**Electroacoustics – Simulators of human head and ear –
Part 7: Head and torso simulator for the measurement of hearing aids**

IECNORM.COM : Click to view the full PDF of IEC TS 60318-7:2011



THIS PUBLICATION IS COPYRIGHT PROTECTED

Copyright © 2011 IEC, Geneva, Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either IEC or IEC's member National Committee in the country of the requester.

If you have any questions about IEC copyright or have an enquiry about obtaining additional rights to this publication, please contact the address below or your local IEC member National Committee for further information.

Droits de reproduction réservés. Sauf indication contraire, aucune partie de cette publication ne peut être reproduite ni utilisée sous quelque forme que ce soit et par aucun procédé, électronique ou mécanique, y compris la photocopie et les microfilms, sans l'accord écrit de la CEI ou du Comité national de la CEI du pays du demandeur.

Si vous avez des questions sur le copyright de la CEI ou si vous désirez obtenir des droits supplémentaires sur cette publication, utilisez les coordonnées ci-après ou contactez le Comité national de la CEI de votre pays de résidence.

IEC Central Office
3, rue de Varembe
CH-1211 Geneva 20
Switzerland
Email: inmail@iec.ch
Web: www.iec.ch

About IEC publications

The technical content of IEC publications is kept under constant review by the IEC. Please make sure that you have the latest edition, a corrigenda or an amendment might have been published.

- Catalogue of IEC publications: www.iec.ch/searchpub

The IEC on-line Catalogue enables you to search by a variety of criteria (reference number, text, technical committee,...). It also gives information on projects, withdrawn and replaced publications.

- IEC Just Published: www.iec.ch/online_news/justpub

Stay up to date on all new IEC publications. Just Published details twice a month all new publications released. Available on-line and also by email.

- Electropedia: www.electropedia.org

The world's leading online dictionary of electronic and electrical terms containing more than 20 000 terms and definitions in English and French, with equivalent terms in additional languages. Also known as the International Electrotechnical Vocabulary online.

- Customer Service Centre: www.iec.ch/webstore/custserv

If you wish to give us your feedback on this publication or need further assistance, please visit the Customer Service Centre FAQ or contact us:

Email: csc@iec.ch
Tel.: +41 22 919 02 11
Fax: +41 22 919 03 00

TECHNICAL SPECIFICATION

**Electroacoustics – Simulators of human head and ear –
Part 7: Head and torso simulator for the measurement of hearing aids**

INTERNATIONAL
ELECTROTECHNICAL
COMMISSION

PRICE CODE



ICS 17.140.50

ISBN 978-2-88912-379-7

CONTENTS

FOREWORD.....	3
INTRODUCTION.....	5
1 Scope.....	6
2 Normative references	6
3 Terms and definitions	6
4 Construction.....	11
4.1 General.....	11
4.2 Geometrical dimensions of the manikin	11
4.2.1 Torso.....	11
4.2.2 Head	18
4.2.3 Pinna.....	24
4.2.4 Ear simulator.....	28
4.2.5 Materials	29
4.2.6 Markings	29
4.2.7 Tolerances	29
4.3 Acoustical characteristics of the manikin.....	29
4.3.1 Free field frequency response.....	29
4.3.2 Tolerances	29
4.3.3 Openings.....	30
5 Calibration.....	30
5.1 Atmospheric reference conditions.....	30
5.2 Calibration method	30
5.2.1 General	30
5.2.2 Test space and measurement equipment.....	30
5.2.3 Measurement of sound pressure level	31
5.2.4 Alignment of manikin azimuth and elevation	31
5.2.5 Test for sound leakage	31
6 Maximum permitted expanded uncertainty of measurements	32
Annex A (informative) Ear canal sound pressure ratio.....	34
Bibliography.....	35
Figure 1 – Manikin geometrical references.....	9
Figure 2 – Coordinate scheme for azimuth and elevation angles	10
Figure 3 – Illustration of manikin head and torso dimensions	12
Figure 4 – Cross-sections of torso (tolerance ± 4 mm).....	17
Figure 5 – Cross-sections of head (tolerance $\pm 2,5$ mm)	23
Figure 6 – Illustration of manikin pinna dimensions	24
Figure 7 – Cross-sections of right pinna (tolerance $\pm 1,5$ mm).....	28
Table 1 – Head and torso dimensions for the manikin and average human data.....	12
Table 2 – Pinna dimensions for the manikin	24
Table 3 – Free field frequency response of the manikin	32
Table 4 – Values of $U_{\max}$ for basic measurements	33
Table A.1 – Ear canal sound pressure ratio	34

INTERNATIONAL ELECTROTECHNICAL COMMISSION

**ELECTROACOUSTICS –
SIMULATORS OF HUMAN HEAD AND EAR –****Part 7: Head and torso simulator
for the measurement of hearing aids**

FOREWORD

- 1) The International Electrotechnical Commission (IEC) is a worldwide organization for standardization comprising all national electrotechnical committees (IEC National Committees). The object of IEC is to promote international co-operation on all questions concerning standardization in the electrical and electronic fields. To this end and in addition to other activities, IEC publishes International Standards, Technical Specifications, Technical Reports, Publicly Available Specifications (PAS) and Guides (hereafter referred to as "IEC Publication(s)"). Their preparation is entrusted to technical committees; any IEC National Committee interested in the subject dealt with may participate in this preparatory work. International, governmental and non-governmental organizations liaising with the IEC also participate in this preparation. IEC collaborates closely with the International Organization for Standardization (ISO) in accordance with conditions determined by agreement between the two organizations.
- 2) The formal decisions or agreements of IEC on technical matters express, as nearly as possible, an international consensus of opinion on the relevant subjects since each technical committee has representation from all interested IEC National Committees.
- 3) IEC Publications have the form of recommendations for international use and are accepted by IEC National Committees in that sense. While all reasonable efforts are made to ensure that the technical content of IEC Publications is accurate, IEC cannot be held responsible for the way in which they are used or for any misinterpretation by any end user.
- 4) In order to promote international uniformity, IEC National Committees undertake to apply IEC Publications transparently to the maximum extent possible in their national and regional publications. Any divergence between any IEC Publication and the corresponding national or regional publication shall be clearly indicated in the latter.
- 5) IEC itself does not provide any attestation of conformity. Independent certification bodies provide conformity assessment services and, in some areas, access to IEC marks of conformity. IEC is not responsible for any services carried out by independent certification bodies.
- 6) All users should ensure that they have the latest edition of this publication.
- 7) No liability shall attach to IEC or its directors, employees, servants or agents including individual experts and members of its technical committees and IEC National Committees for any personal injury, property damage or other damage of any nature whatsoever, whether direct or indirect, or for costs (including legal fees) and expenses arising out of the publication, use of, or reliance upon, this IEC Publication or any other IEC Publications.
- 8) Attention is drawn to the Normative references cited in this publication. Use of the referenced publications is indispensable for the correct application of this publication.
- 9) Attention is drawn to the possibility that some of the elements of this IEC Publication may be the subject of patent rights. IEC shall not be held responsible for identifying any or all such patent rights.

The main task of IEC technical committees is to prepare International Standards. In exceptional circumstances, a technical committee may propose the publication of a technical specification when

- the required support cannot be obtained for the publication of an International Standard, despite repeated efforts, or
- the subject is still under technical development or where, for any other reason, there is the future but no immediate possibility of an agreement on an International Standard.

Technical specifications are subject to review within three years of publication to decide whether they can be transformed into International Standards.

IEC/TS 60318-7, which is a technical specification, has been prepared by IEC technical committee 29: Electroacoustics.

The text of this technical specification is based on the following documents:

Enquiry draft	Report on voting
29/716/DTS	29/729A/RVC

Full information on the voting for the approval of this technical specification can be found in the report on voting indicated in the above table.

This publication has been drafted in accordance with the ISO/IEC Directives, Part 2.

A list of all parts of the IEC 60318 series, published under the general title *Electroacoustics – Simulators of human head and ear*, can be found on the IEC website.

The committee has decided that the contents of this publication will remain unchanged until the stability date indicated on the IEC web site under "<http://webstore.iec.ch>" in the data related to the specific publication. At this date, the publication will be

- transformed into an International standard,
- reconfirmed,
- withdrawn,
- replaced by a revised edition, or
- amended.

A bilingual version of this document may be issued at a later date.

INTRODUCTION

This technical specification describes a head and torso simulator for hearing aid measurements. It has been developed as a revision of IEC/TR 60959 (1990). The main changes, as compared to the technical report, are the insertion of maximum permitted expanded measurement uncertainties and additional references in the Bibliography. A future IEC Standard which will include additional models of head and torso simulators for hearing aid measurements is planned.

IECNORM.COM : Click to view the full PDF of IEC TS 60318-7:2011

ELECTROACOUSTICS – SIMULATORS OF HUMAN HEAD AND EAR –

Part 7: Head and torso simulator for the measurement of hearing aids

1 Scope

This part of IEC 60318 describes a head and torso simulator (manikin) intended for the measurement of air-conduction hearing aids in the frequency range from 100 Hz to 10 000 Hz. The device consists of a head mounted on a torso that extends to the waist. The head is equipped with simulated pinnae and with cylindrical cavities having acoustic impedance terminations and microphones located at positions corresponding to those of the eardrums in a median human adult. It has been designed to provide acoustic diffraction similar to that encountered around the median human head and torso.

The device with its present pinna simulator, however, is not suitable for the measurement of all types of hearing aids. For example, most in-the-ear (ITE) and completely-in-the-canal (CIC) hearing aids cannot be measured correctly.

The manikin is specified in terms of both, its geometrical dimensions and its acoustical properties.

NOTE 1 Measurement results obtained with a manikin may differ substantially from similar results obtained on an individual person, due to anatomical variations.

NOTE 2 The median values of the human head and torso were drawn from the population samples described in [5]¹.

NOTE 3 It is acknowledged that devices conforming to this part of IEC 60318 are also used as the basis for applications extending beyond this Scope. In such cases it is recommended that any design variations that are necessary are documented, and that a statistical analysis of the measurement data be carried out to determine the level of repeatability that can be achieved. It will also be necessary to consider the relevance of the measurements made with the head and torso simulator to the application in question.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

IEC 60318-4, *Simulators of human head and ear – Part 4: Occluded-ear simulator for the measurement of earphones coupled to the ear by means of ear inserts*

ISO/IEC Guide 98-3, *Uncertainty of measurement – Part 3: Guide to the expression of uncertainty in measurement* (GUM:1995)

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply. Reference is also made to Figure 1 and Figure 2.

¹ Numbers in square brackets refer to the Bibliography.

3.1

manikin

head and torso simulator extending downward from the top of the head to the waist and designed to simulate the acoustic diffraction produced by a median adult human head and torso

NOTE The head includes two pinna simulators, and contains at least one ear simulator.

3.2

pinna simulator

device which has the approximate shape and dimensions of a median adult human pinna

3.3

ear simulator

device for measuring the acoustic output of sound sources where the sound pressure is measured by a calibrated microphone coupled to the source so that the overall acoustic impedance of the device approximates that of the normal human ear at a given location and in a given frequency band

NOTE In this technical specification it comprises an ear canal extension and an occluded ear simulator.

3.4

occluded ear simulator

ear simulator which approximates the acoustic transfer impedance of the inner part of the ear canal, from the tip of an ear insert to the eardrum

NOTE An occluded ear simulator is standardised in IEC 60318-4

3.5

ear canal extension

device that provides a connection between the ear canal of an occluded ear simulator and the aperture of a device simulating the concha

3.6

reference plane of the occluded ear simulator

plane perpendicular to the axis of the ear canal, at the junction between the occluded ear simulator and the ear canal extension

3.7

reference point of the manikin

point bisecting the line joining the centres of the openings of the ear canals (at the junction between concha and ear canal)

3.8

plane of symmetry of the manikin

virtual plane passing through the reference point of the manikin that divides the left and right portions of the manikin into symmetrical halves, left and right to be interpreted as for the human torso (see Figure 1)

NOTE No real human is perfectly symmetrical.

3.9

axis of rotation of the manikin

straight line about which the manikin can be rotated, passing through the reference point of the manikin and lying in the plane of symmetry of the manikin, and having a direction that would be vertical if the manikin were mounted in a position corresponding to that of a standing person (see Figure 1)

3.10

reference plane of the manikin

plane perpendicular to the axis of rotation that contains the reference point of the manikin

3.11

test point

reproducible position in the test space at which the sound pressure level is measured with the manikin absent and at which the reference point of the manikin is to be located for test purposes

3.12

test axis

line joining the test point and the centre of the sound source (see Figure 2)

3.13

test plane

plane perpendicular to the test axis and containing the test point

3.14

azimuth angle of sound incidence

θ

angle between the plane of symmetry of the manikin (see Figure 2) and the plane defined by the axis of rotation and the test axis; when the manikin faces the sound source, the azimuth angle of sound incidence is defined as 0°

NOTE When the right ear of the manikin faces the sound source, the angle is defined as $+90^\circ$. When the left ear of the manikin faces the sound source, the angle is defined as $+270^\circ$.


3.15

elevation angle of sound incidence

α


angle between the reference plane of the manikin and the test axis (see Figure 2); when the vertex points towards the sound source, the elevation angle is defined as $+90^\circ$

NOTE When the test axis lies in the reference plane, the elevation angle is defined as 0° .

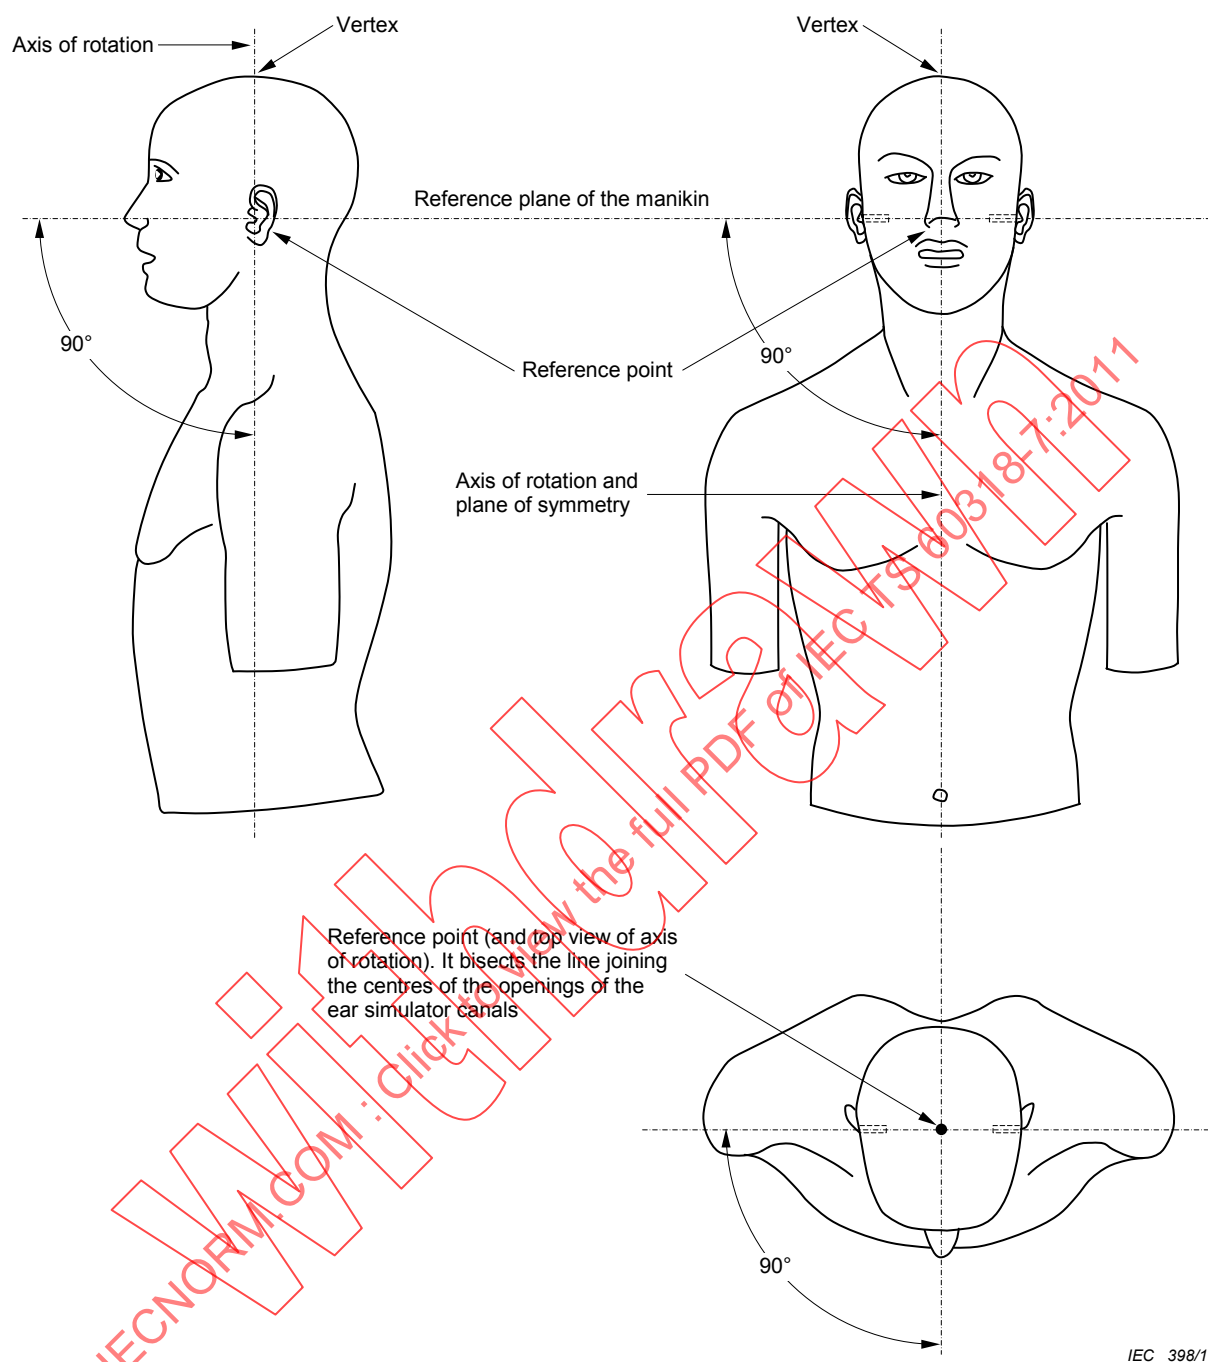

NOTE The reference point is the reference point of the manikin.

Figure 1 – Manikin geometrical references

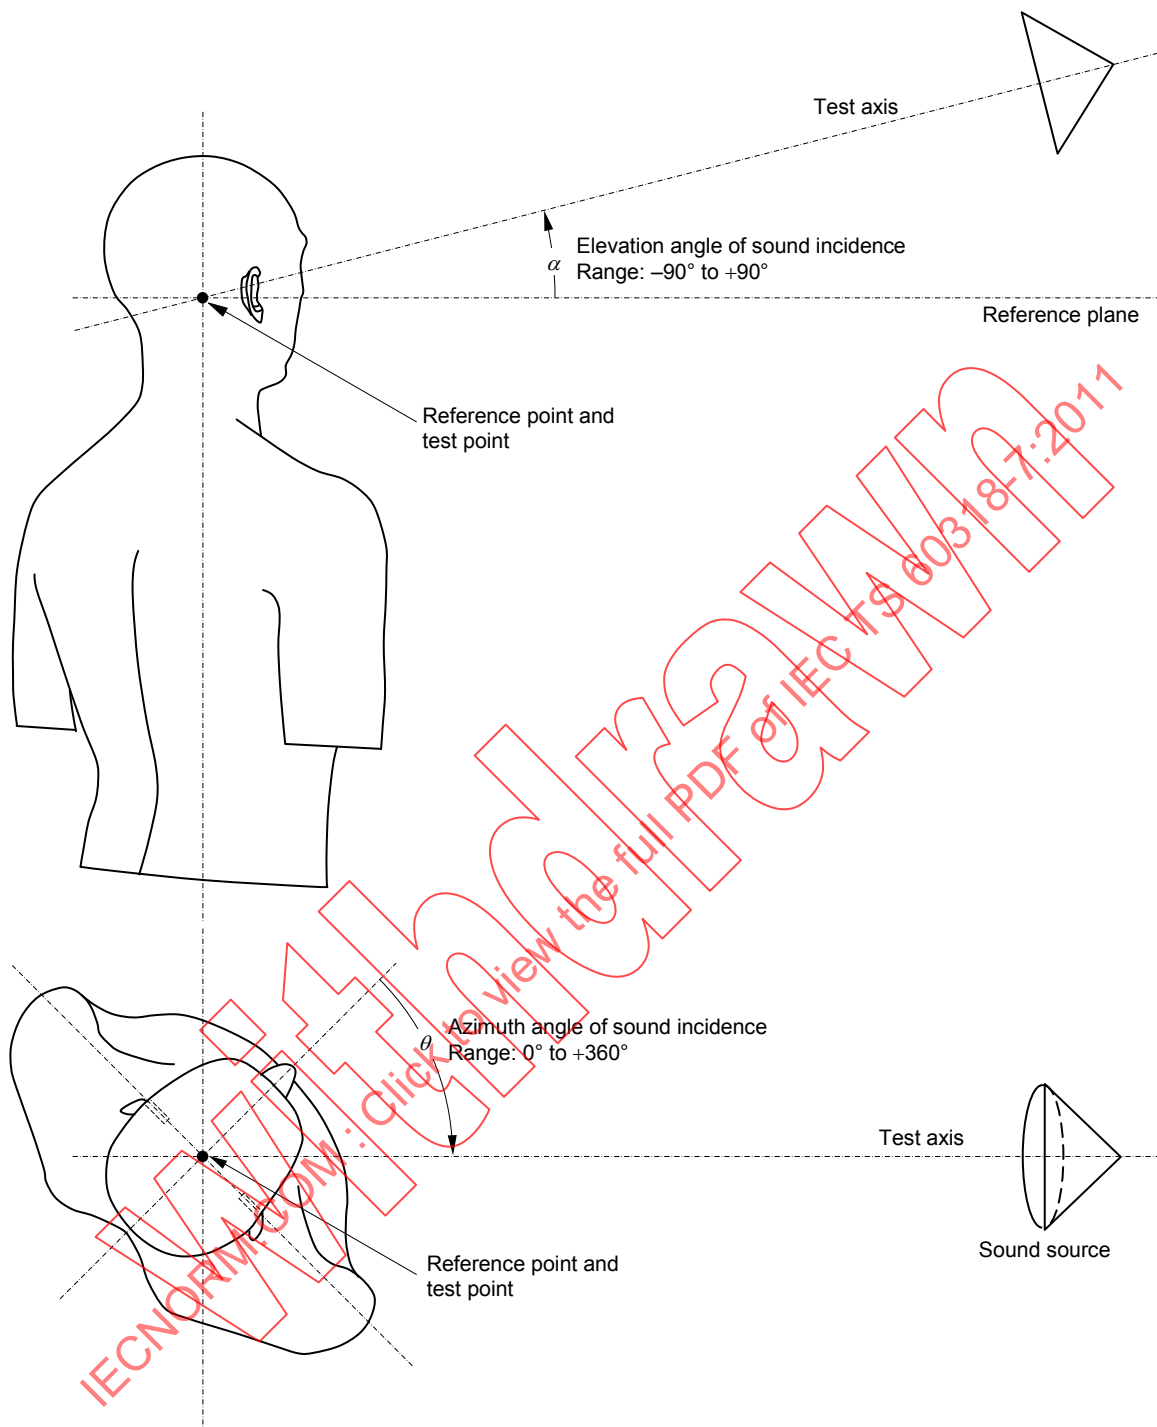

IEC 399/11

NOTE The reference point is the reference point of the manikin.

Figure 2 – Coordinate scheme for azimuth and elevation angles

3.16**reference position of the manikin**

position of the manikin in the test space that meets the following conditions:

- the reference point of the manikin coincides with the test point,
- the azimuth and elevation angles are both equal to zero

3.17**manikin free field frequency response**

difference, as a function of frequency, between the sound pressure level at the ear simulator microphone with the reference point of the manikin at the test point and the sound pressure level at the test point with the manikin absent

3.18**ear canal entrance point****EEP**

point located at the centre of the manikin ear canal at the junction between concha and ear canal extension

3.19**vertical pinna reference axis**

line through the EEP, and parallel to the axis of rotation of the manikin

3.20**horizontal pinna reference axis**

line through the EEP, and parallel to the reference plane of the manikin with an azimuth angle of 90°


NOTE The horizontal pinna reference axis is needed for vertical cross-sections of a pinna simulator, see for instance IEC 60268-7 [1].

4 Construction**4.1 General**

In the following, both the geometrical physical dimensions of the manikin's head, torso and pinnae and the manikin's acoustical characteristics are specified. Where tolerances are specified in this technical specification, these shall be reduced by an amount equal to the actual expanded measurement uncertainty of the test laboratory before deciding if a device conforms to the stated requirement.

4.2 Geometrical dimensions of the manikin**4.2.1 Torso**

4.2.1.1 The principal geometrical dimensions of the manikin torso are illustrated in Figure 3, and listed in Table 1 (for information only). The realization of the torso is specified in 4.2.1.2.

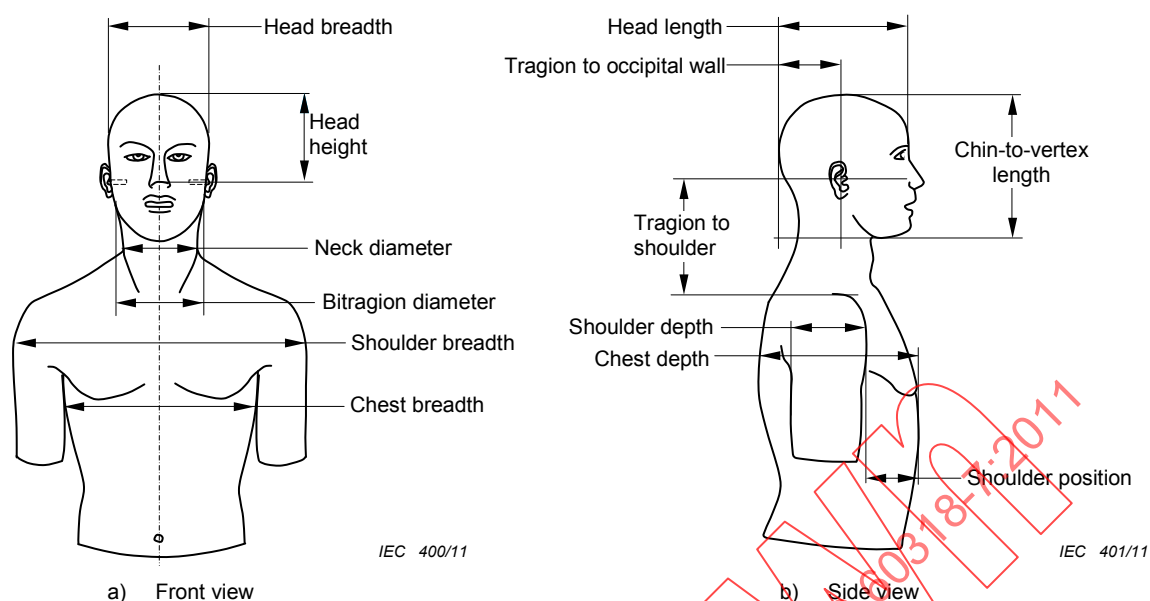

NOTE For position of tracion, see Figure 6.

Figure 3 – Illustration of manikin head and torso dimensions

Table 1 – Head and torso dimensions for the manikin and average human data


Dimension	Manikin (mm)	Average human data [5] (mm)
Head breadth	152	151
Head length	191	188
Head height (tracion to vertex)	125	130
Bitracion diameter	143	139
Tracion to occipital wall	97	98
Tracion to shoulder	175	176
Neck diameter	113	112
Shoulder breadth	440	427
Chest breadth	282	291
Chin to vertex length	224	222
Chest depth	235	--
Shoulder depth	110	--
Shoulder position	80	--

NOTE 1 The data given in Table 1 is for information only.

NOTE 2 In order to be independent of the type of pinna simulator, the tracion sometimes is replaced by the ear canal entrance point (EEP) as reference point of the manikin [5]. In this case the corresponding manikin values are: EEP to vertex 130 mm, EEP to EEP distance 132 mm, EEP to occipital wall 94 mm and EEP to shoulder 170 mm.

4.2.1.2 Cross-sections parallel to the reference plane of the manikin are given in Figures 4a) to 4e). Each cross-section is identified by the distance (in millimetres, negative towards the waist) from the reference plane of the manikin. Circles indicate the position of the axis of rotation of the manikin. Grid lines are spaced 20 mm.

NOTE The torso is symmetrical. Cross-sections are shown only for the top view of the right side. The orientation of the cross-section is such that the front of the head points downwards.

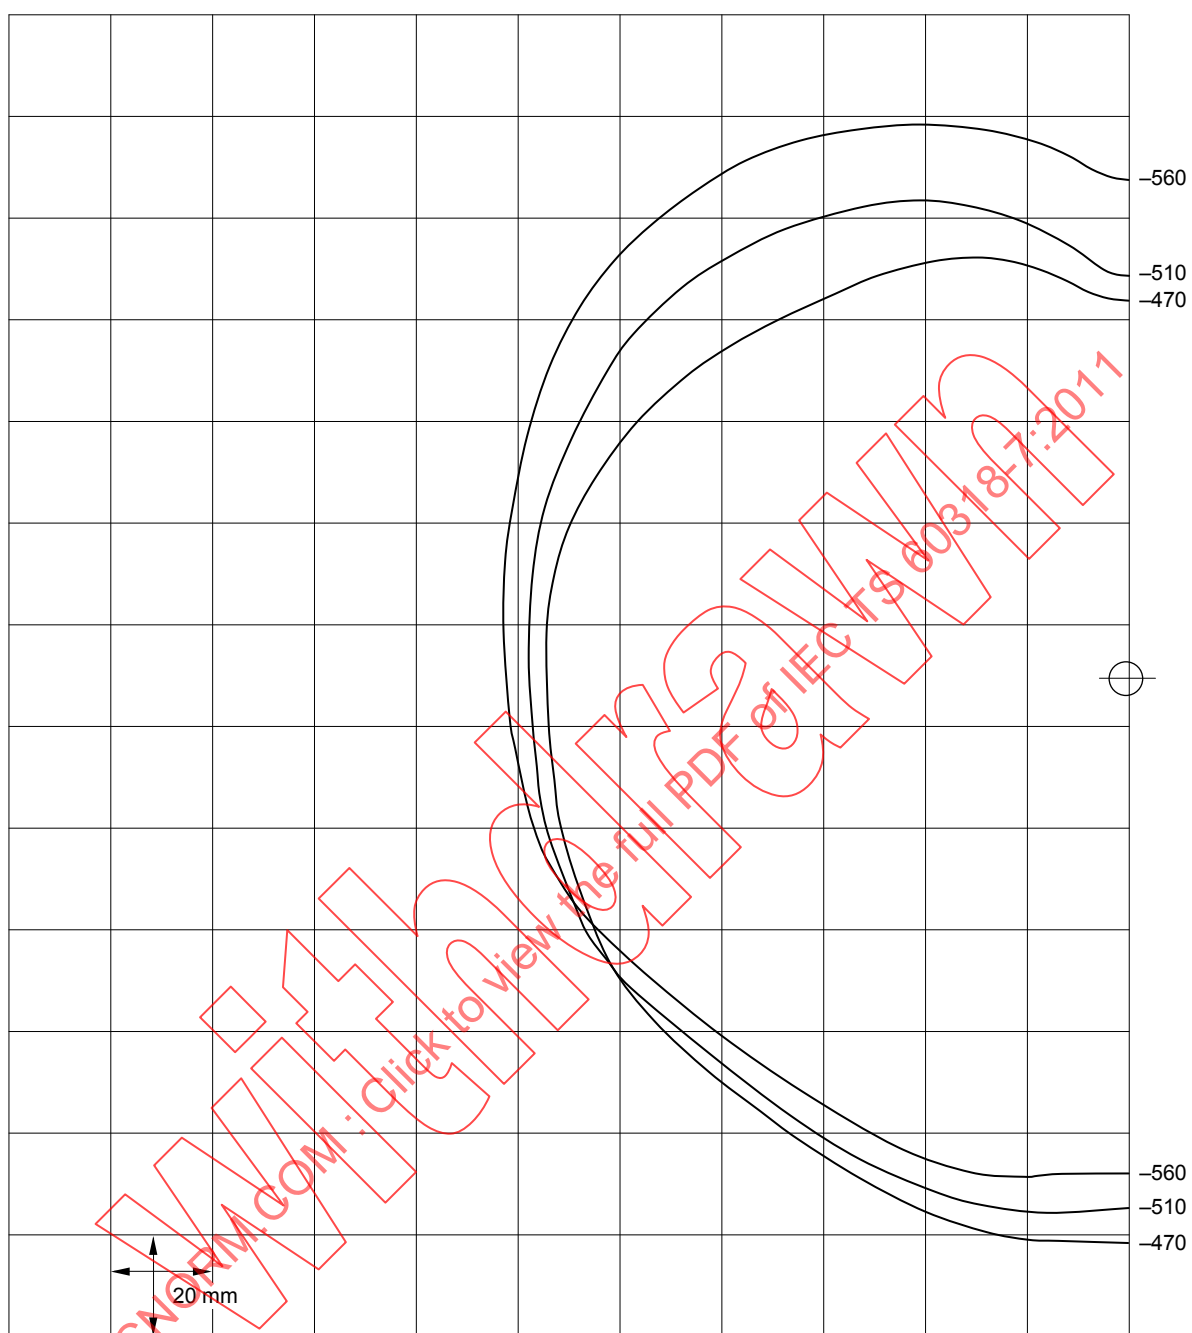


IEC 402/11

NOTE 1 Not to scale, convert grid as dimensioned.

NOTE 2 For detailed information on the graph refer to 4.2.1.2.

4a) Cross-section 1

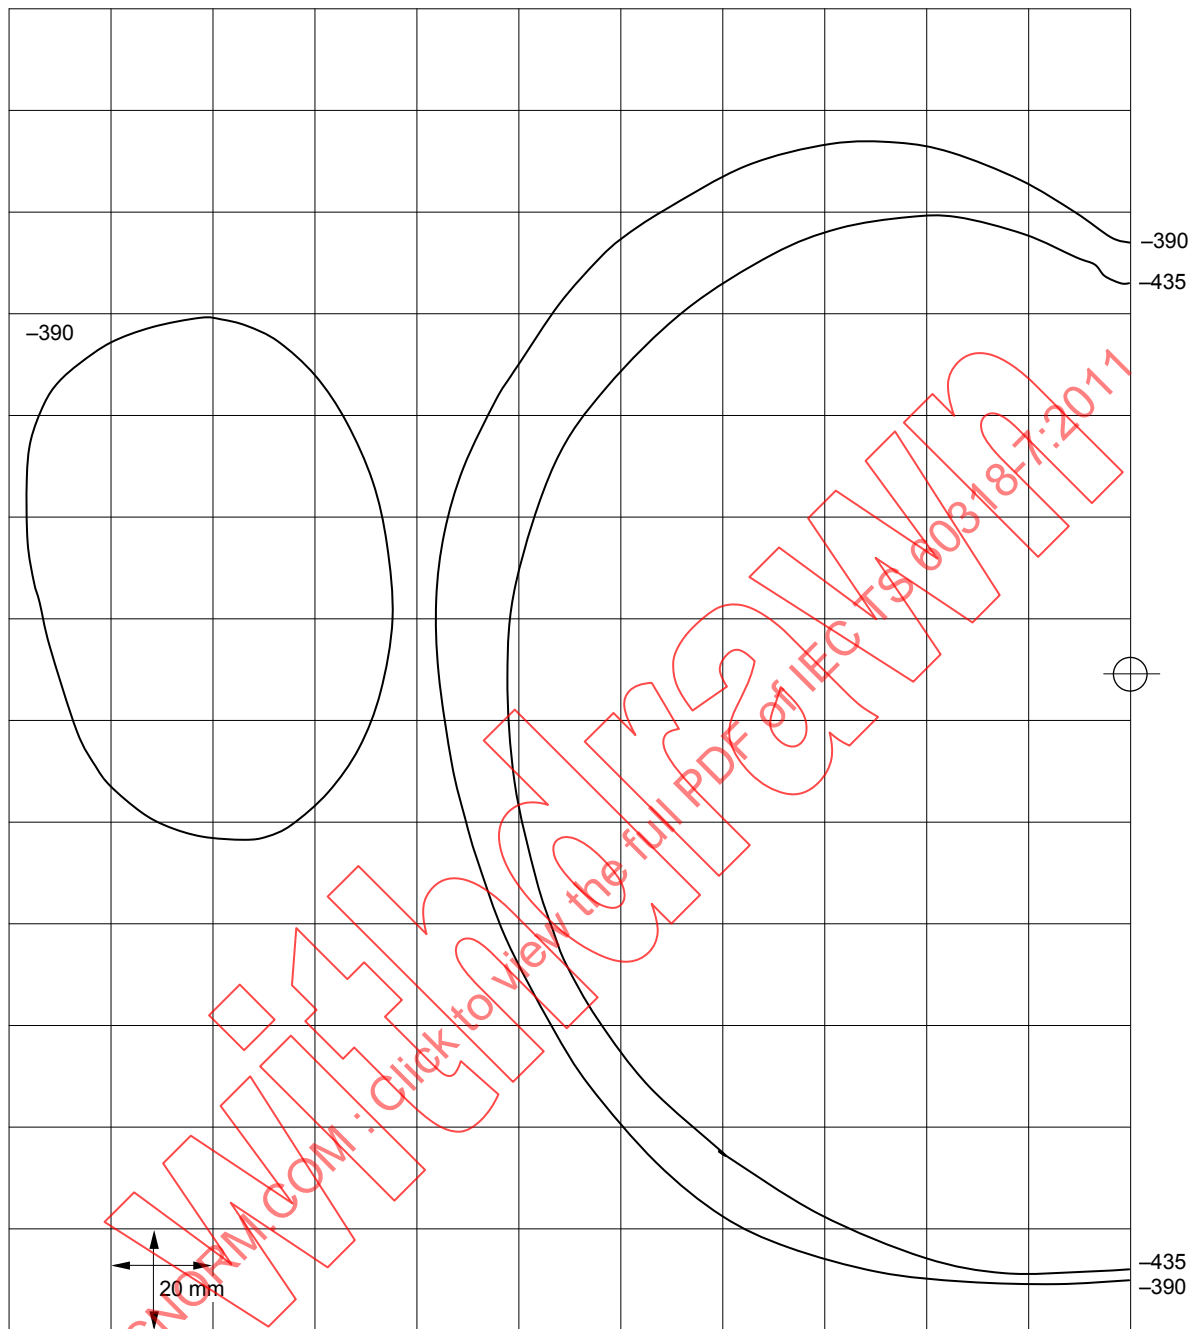


IEC 403/11

NOTE1 Not to scale, convert grid as dimensioned.

NOTE 2 For detailed information on the graph refer to 4.2.1.2.

4b) Cross-section 2

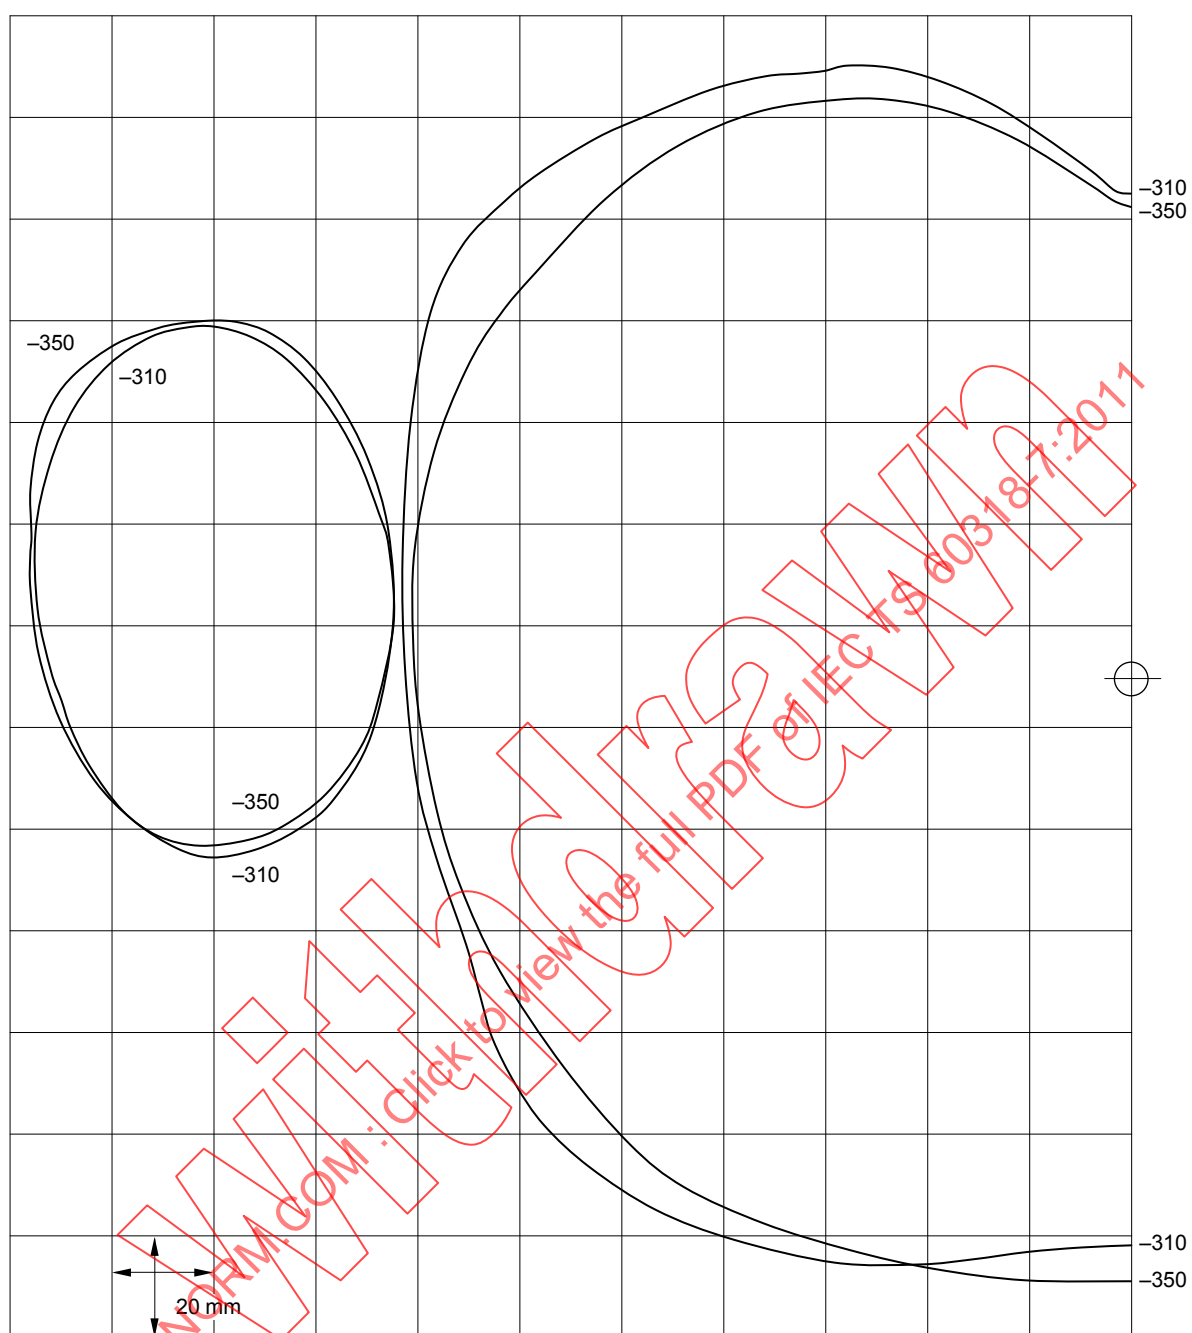


IEC 404/11

NOTE 1 Not to scale, convert grid as dimensioned.

NOTE 2 For detailed information on the graph refer to 4.2.1.2.

4c) Cross-section 3

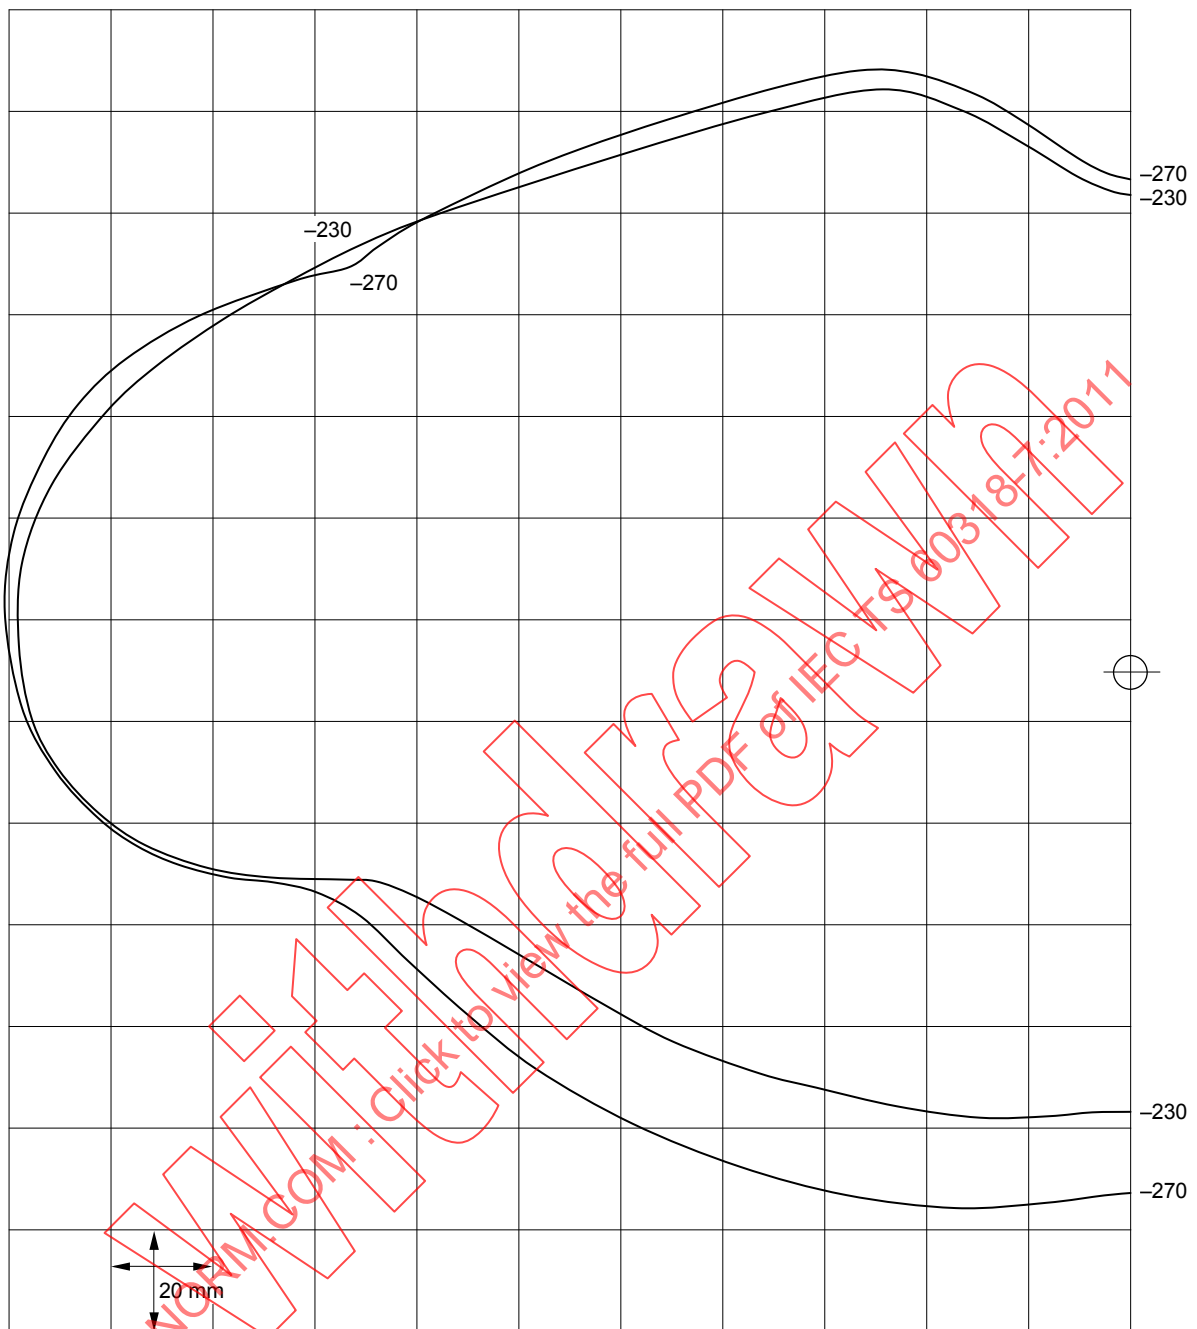


IEC 405/11

NOTE 1 Not to scale, convert grid as dimensioned.

NOTE 2 For detailed information on the graph refer to 4.2.1.2.

4d) Cross-section 4

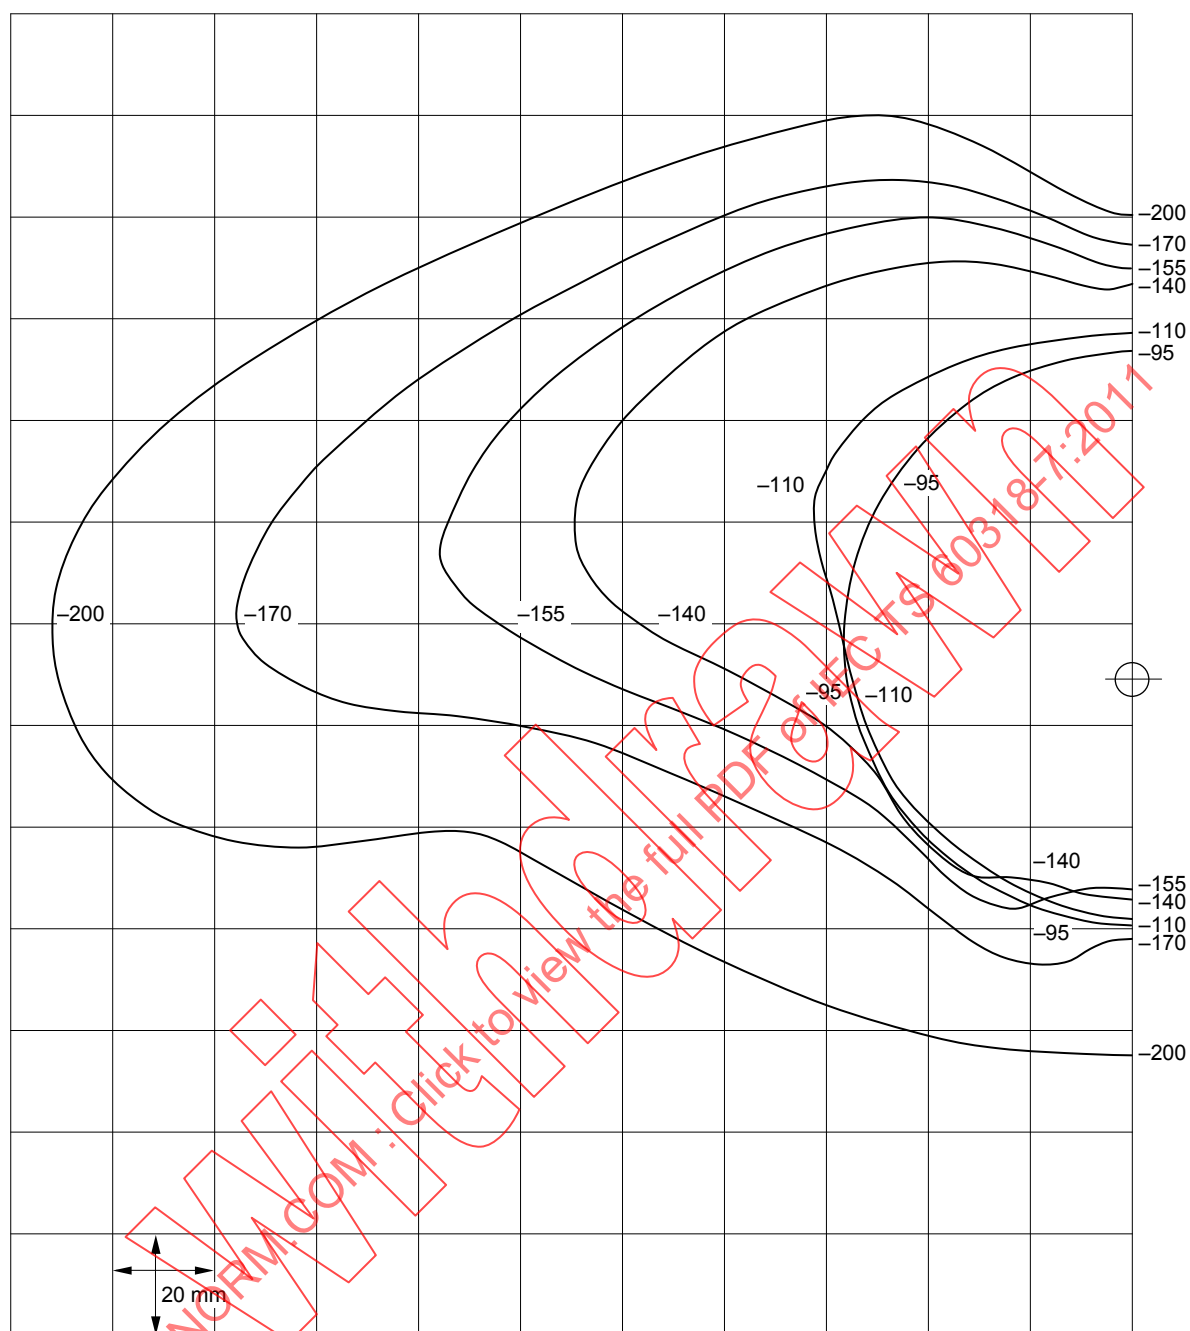

IEC 406/11

NOTE 1 Not to scale, convert grid as dimensioned.

NOTE 2 For detailed information on the graph refer to 4.2.1.2.

4e) Cross-section 5

Figure 4 – Cross-sections of torso (tolerance ± 4 mm)


4.2.2 Head

4.2.2.1 The principal geometrical dimensions of the manikin head are illustrated in Figure 3, and listed in Table 1 (for information only). The realization of the head is specified in 4.2.2.2.

4.2.2.2 Cross-sections parallel to the reference plane of the manikin are given in Figures 5a) to 5e). Each cross-section is identified by the distance (in millimetres, positive towards the vertex, negative towards the waist) from the reference plane of the manikin. Circles indicate the position of the axis of rotation of the manikin. The dot in Figures 5b) to 5d) indicates the position of the ear canal entrance point (EEP). The vertical pinna reference axis is used as a reference for location of the pinna cross-sections. Grid lines are spaced 20 mm.

NOTE The head is symmetrical; cross-sections are shown only for the top view of the right side. The orientation of the cross-section is such that the front of the head points downwards.

IECNORM.COM : Click to view the full PDF of IEC TS 60318-7:2017

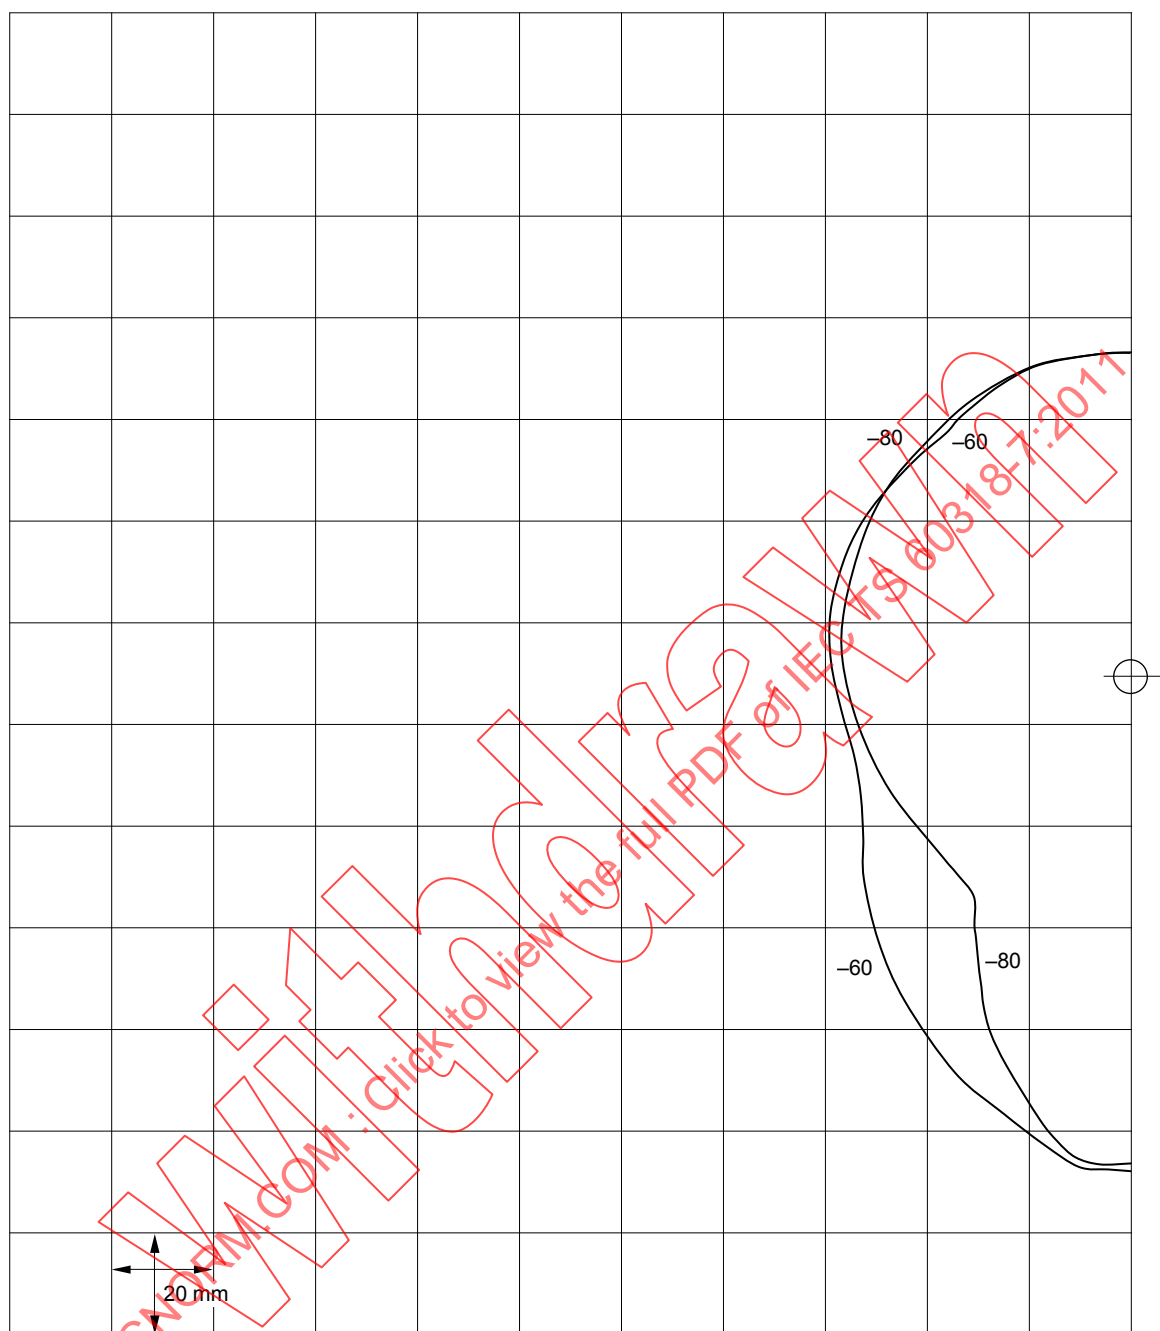


IEC 407/11

NOTE 1 Not to scale, convert grid as dimensioned.

NOTE 2 For detailed information on the graph refer to 4.2.2.2.

5a) Cross-section 1

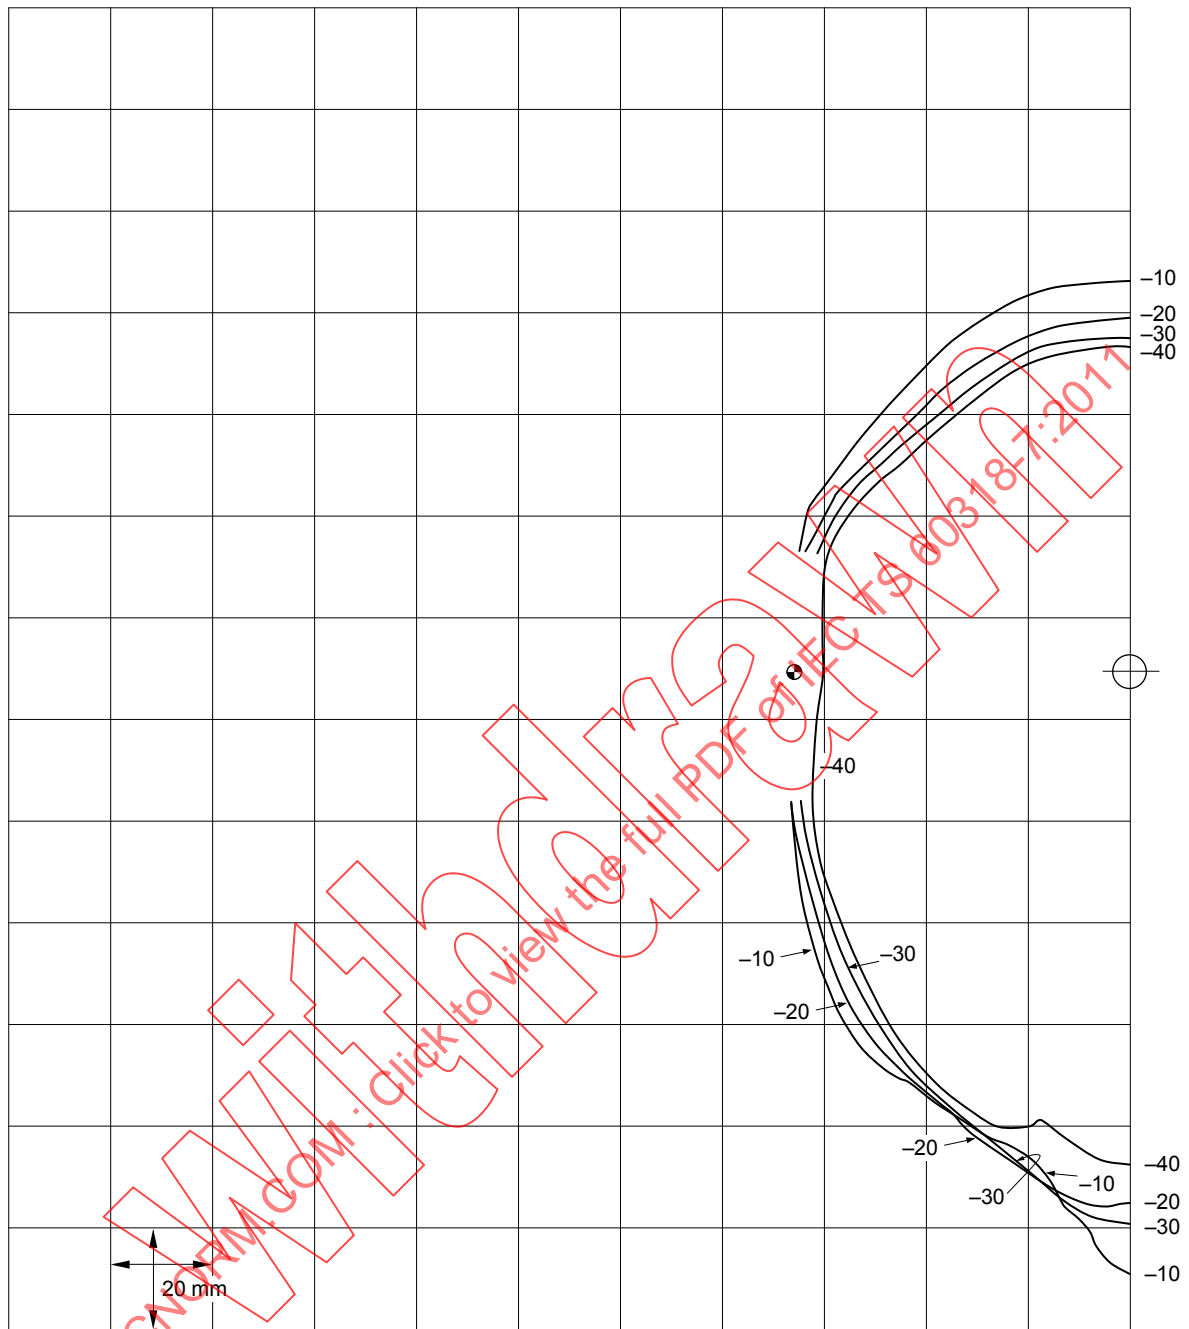


IEC 408/11

NOTE 1 Not to scale, convert grid as dimensioned.

NOTE 2 For detailed information on the graph refer to 4.2.2.2.

NOTE 3 For missing segments refer to Figures 7a) to 7c).

5b) Cross-section 2

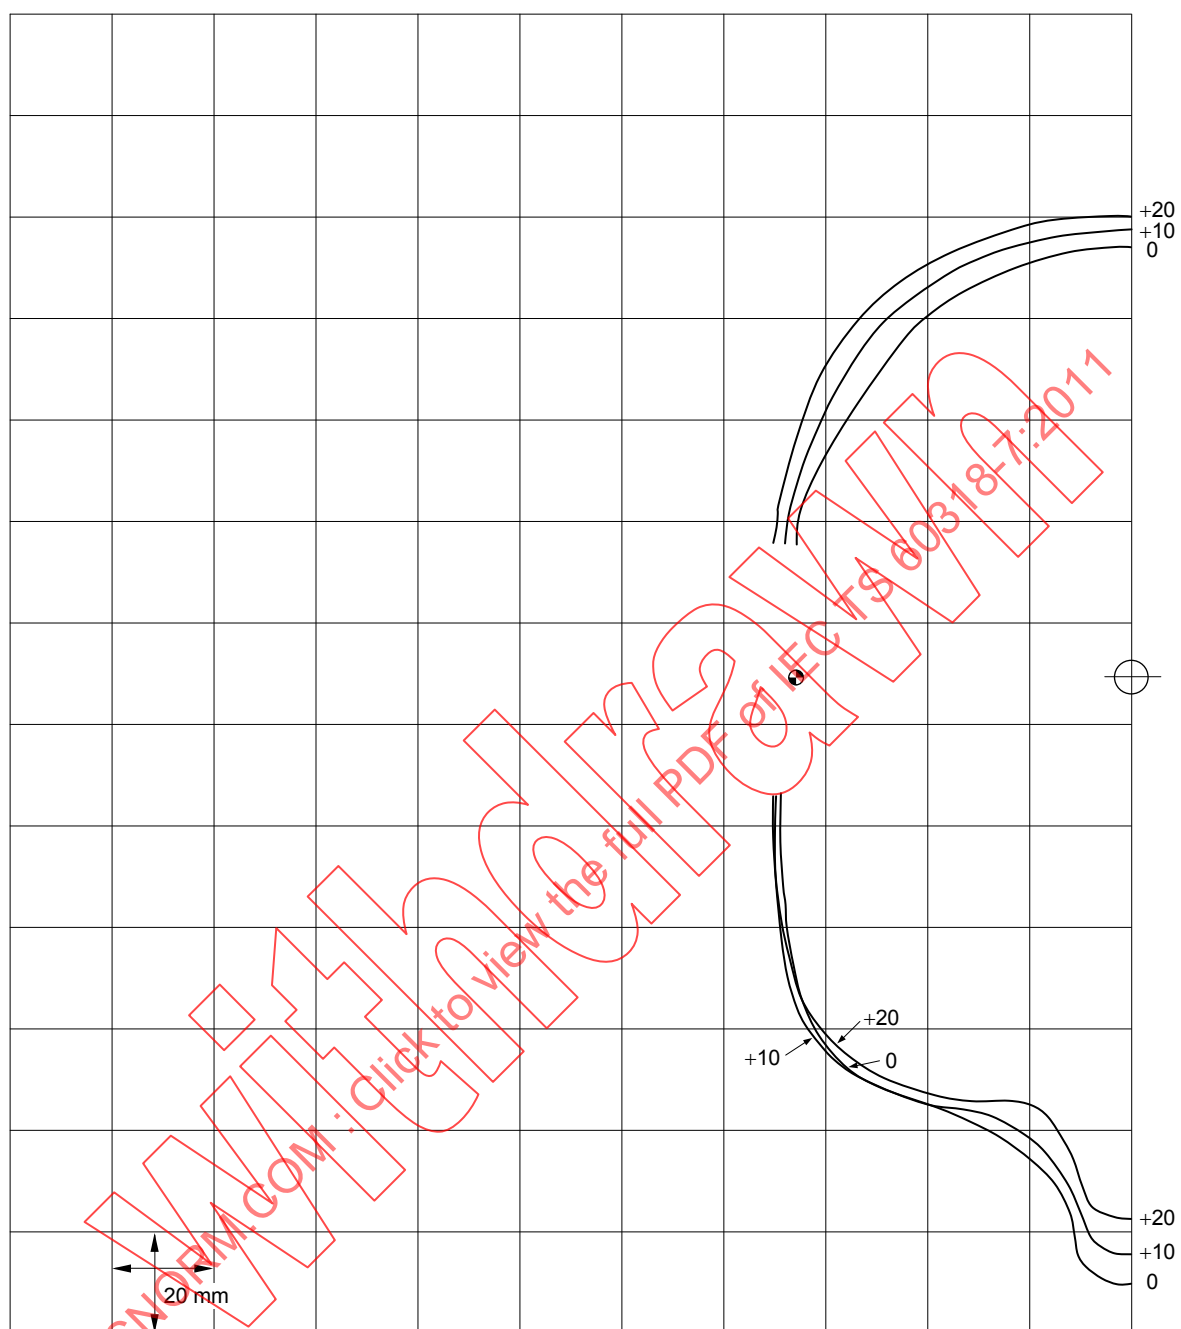


IEC 409/11

NOTE 1 Not to scale, convert grid as dimensioned.

NOTE 2 For detailed information on the graph refer to 4.2.2.2.

NOTE 3 For missing segments refer to Figures 7a) to 7c).

5c) Cross-section 3

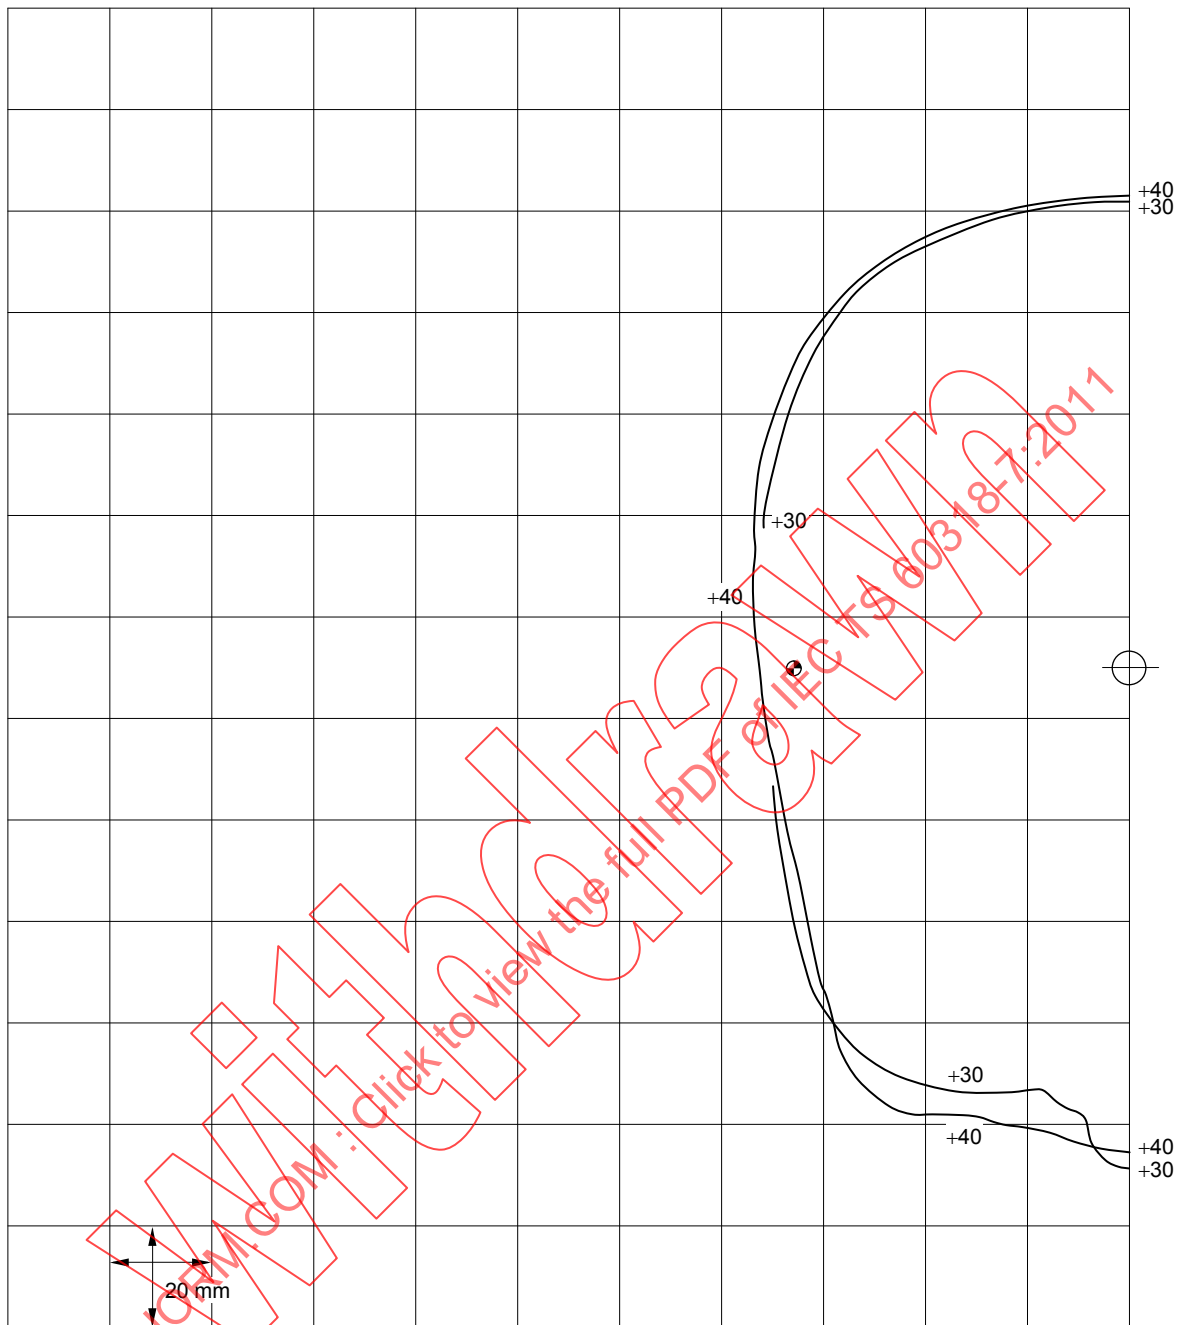


IEC 410/11

NOTE 1 Not to scale, convert grid as dimensioned.

NOTE 2 For detailed information on the graph refer to 4.2.2.2.

NOTE 3 For missing segments refer to Figures 7a) to 7c).

5d) Cross-section 4

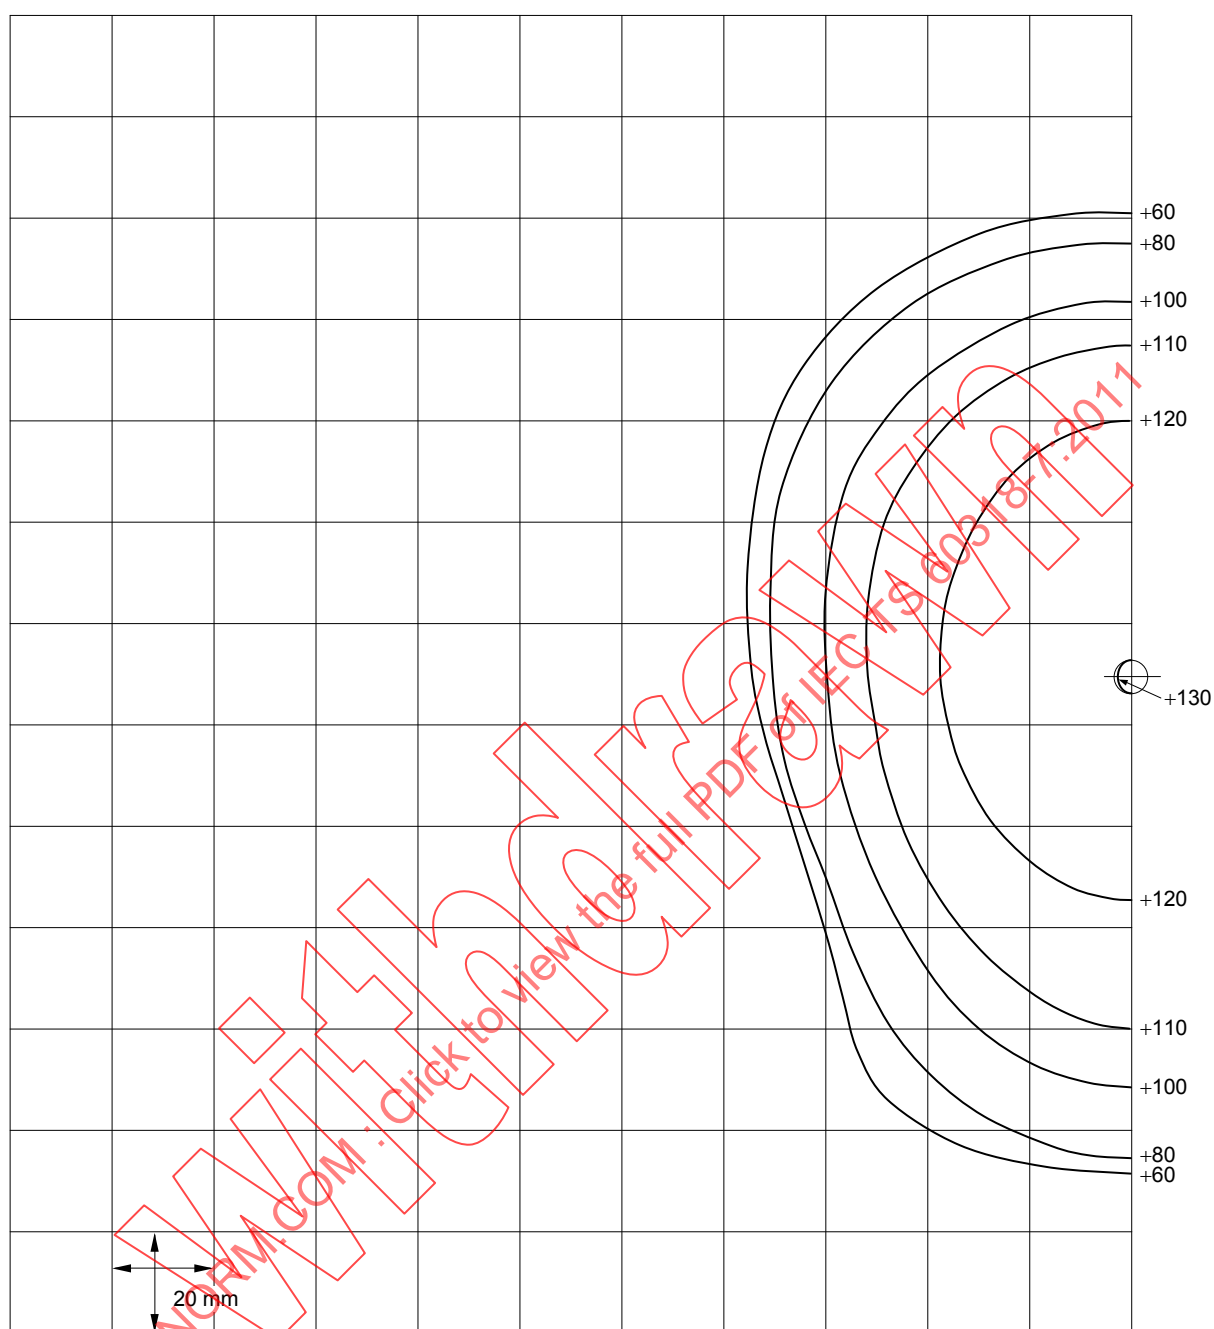

IEC 411/11

NOTE 1 Not to scale, convert grid as dimensioned.


NOTE 2 For detailed information on the graph refer to 4.2.2.2.

5e) Cross-section 5

Figure 5 – Cross-sections of head (tolerance $\pm 2,5$ mm)

4.2.3 Pinna

4.2.3.1 The principal geometrical dimensions and orientation of the simulated pinna are illustrated in Figure 6, and listed in Table 2 (for information only). The realization of the simulated pinna is specified in 4.2.3.2.

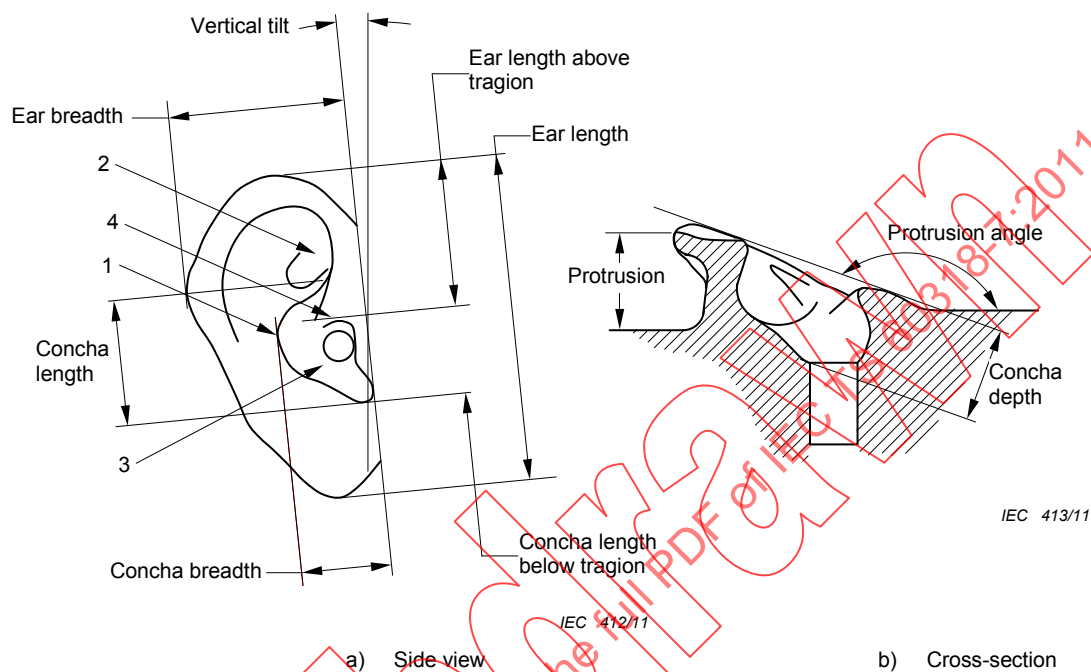

Key

1. Anti-helix
2. Crus of helix
3. Concha
4. Tragon

Figure 6 – Illustration of manikin pinna dimensions

Table 2 – Pinna dimensions for the manikin

Dimension	Manikin (mm and °)
Ear length	66
Ear length above tragon	30
Ear breadth	37
Ear protrusion	23
Ear protrusion angle	160°
Vertical tilt front view	10°
Vertical tilt side view	6°
Concha length	28
Concha length below tragon	20
Concha breadth	23
Concha breadth, tragon to helix	23
Concha depth	15

NOTE The data given in Table 2 is for information only.

4.2.3.2 Cross-sections parallel to the reference plane of the manikin are given in Figures 7a) to 7c). Each cross-section is identified by the distance (in millimetres, positive towards the vertex, negative towards the waist) from the section plane to the reference plane of the manikin.


The dots indicate the position of the vertical pinna reference axis (see 4.2.2.2). The grid lines are spaced 10 mm.

NOTE 1 Figures 7a) to 7c) show cross-sections for the top view of the right pinna. The left pinna is determined as a mirror image of the right pinna.

NOTE 2 The relation between dimensional details and acoustical performance of the pinna are at present only partially understood, and minor adjustments of concha shape, anti-helix, crus of helix, and the location of pinna relative to ear canal may be necessary to conform with the acoustical specifications (see 4.3), particularly at high frequencies.

NOTE 3 The position of the ear simulator relative to the pinna is shown in Figure 7b).

NOTE 4 In addition to the pinna simulator described in this technical specification, there are other types of pinna simulator on the market. These pinna simulators, however, do not fulfill the requirements of Table 3 of this technical specification.

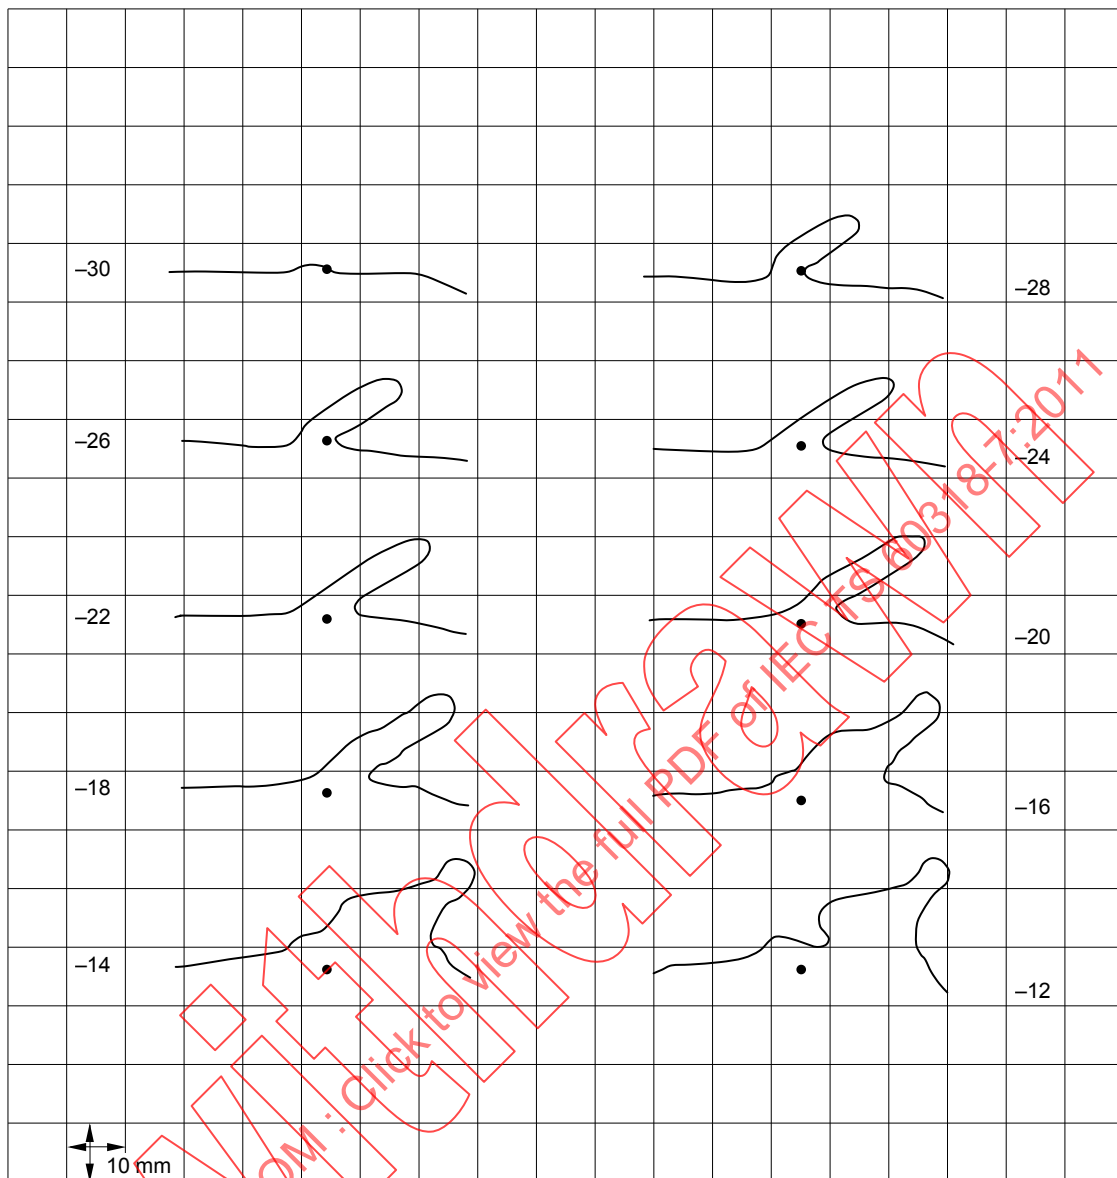


IEC 414/11

NOTE 1 Not to scale, convert grid as dimensioned.

NOTE 2 The orientation of the cross-section is such that the front of the head points leftwards.

NOTE 3 For detailed information on the graph refer to 4.2.3.2.

7a) Cross-section 1

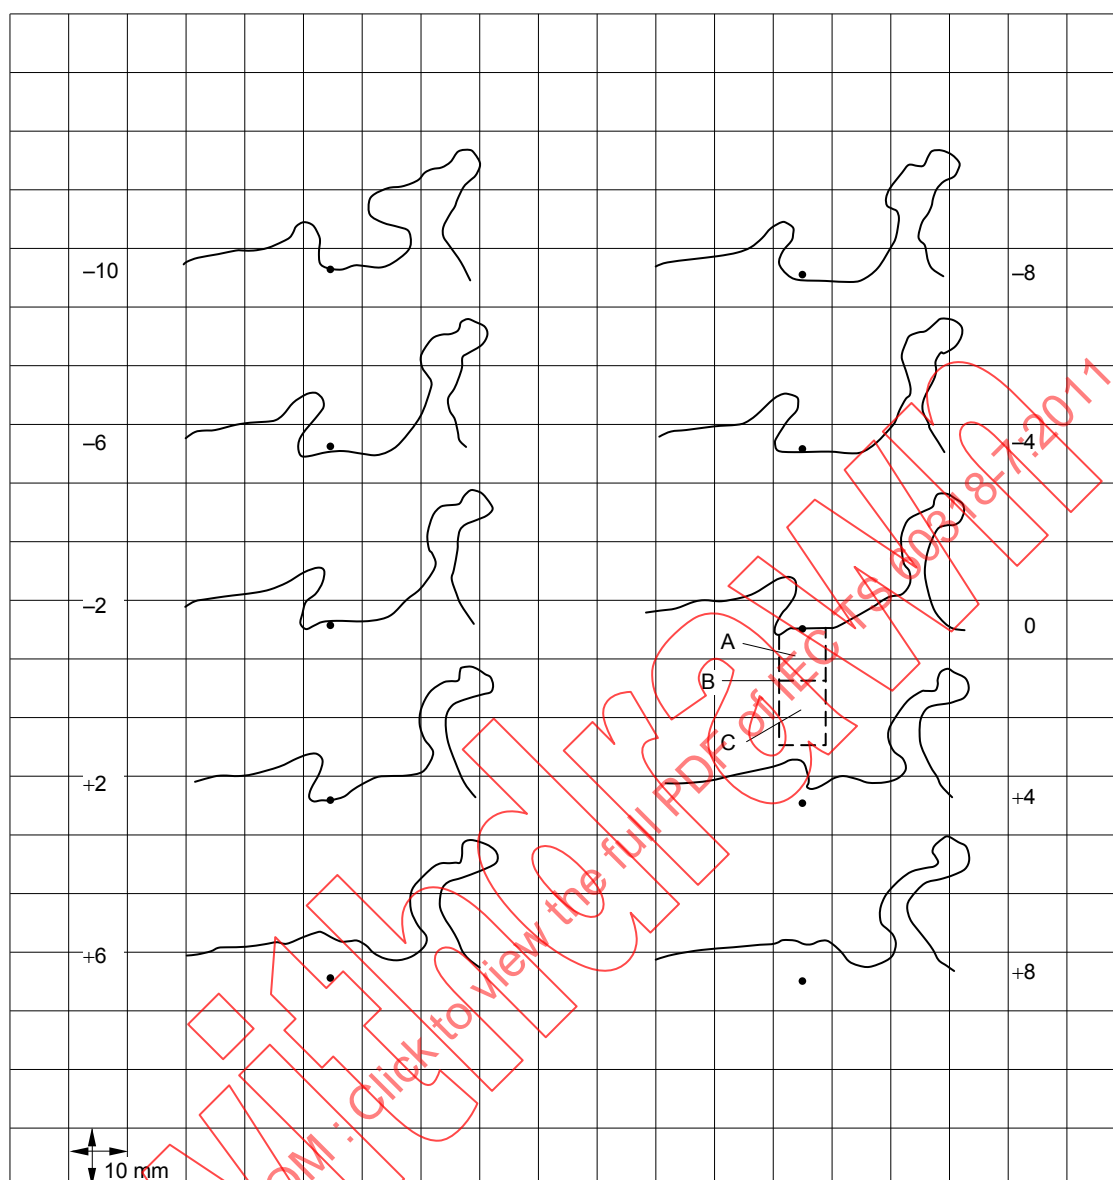

IEC 415/11

Key


- A Ear canal extension
- B Occluded ear simulator reference plane
- C Occluded ear simulator

NOTE 1 Not to scale, convert grid as dimensioned.

NOTE 2 The orientation of the cross-section is such that the front of the head points leftwards.

NOTE 3 For detailed information on the graph refer to 4.2.3.2.

7b) Cross-section 2

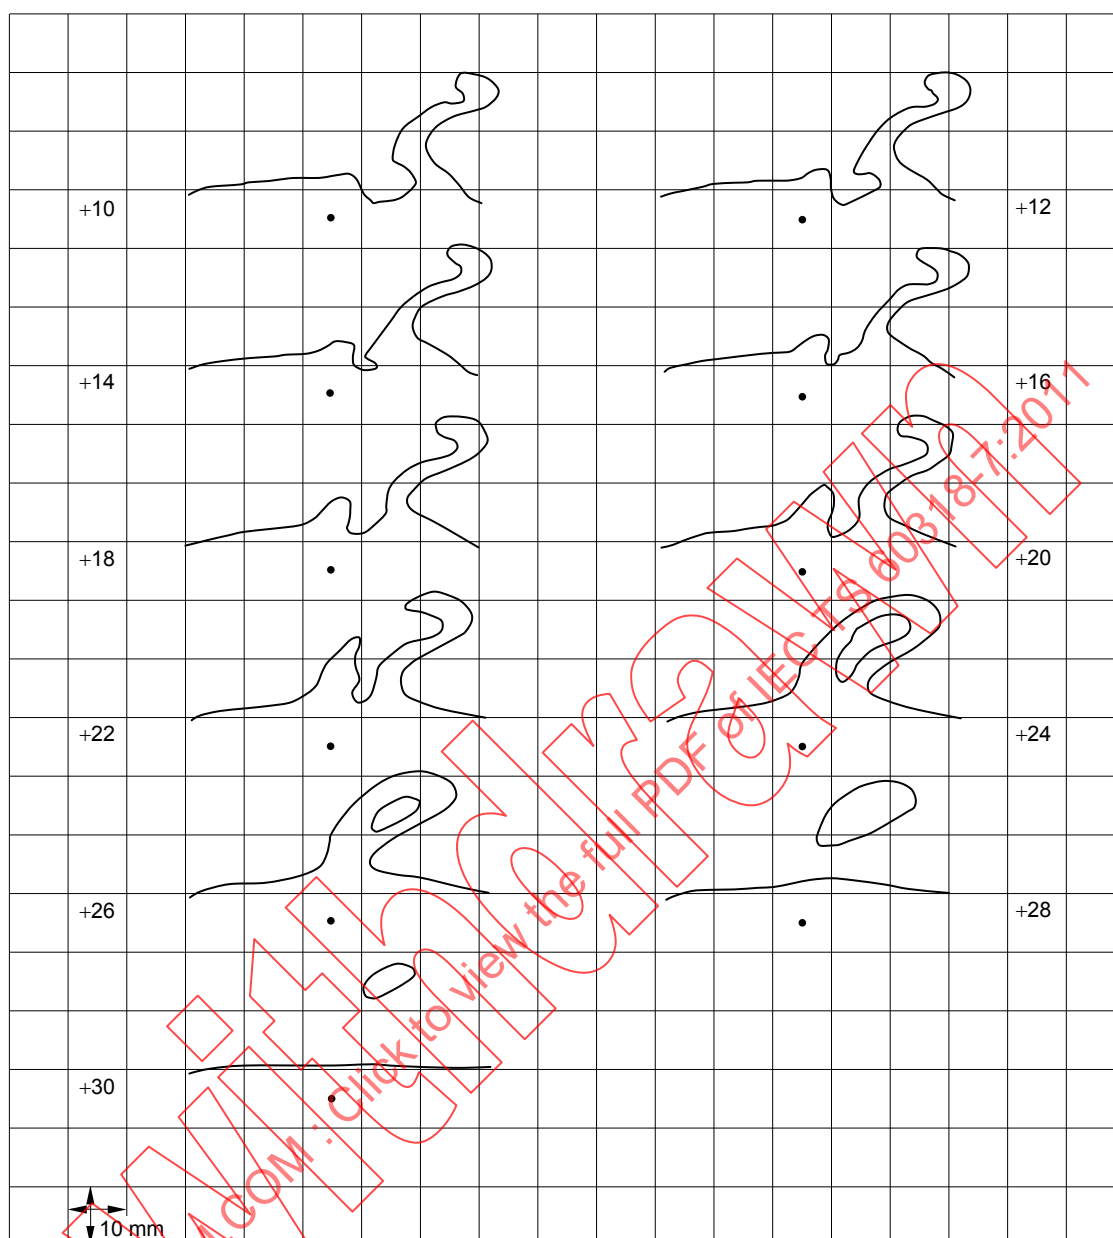

IEC 416/11

NOTE 1 Not to scale, convert grid as dimensioned.

NOTE 2 The orientation of the cross-section is such that the front of the head points leftwards.

NOTE 3 For detailed information on the graph refer to 4.2.3.2.

7c) Cross-section 3

Figure 7 – Cross-sections of right pinna (tolerance $\pm 1,5$ mm)

4.2.4 Ear simulator

The ear simulator shall comprise an occluded ear simulator as described in IEC 60318-4, and an ear canal extension. The ear canal extension shall have a cylindrical form with the length of $8,8 \text{ mm} \pm 0,3 \text{ mm}$ and diameter of $7,5 \text{ mm} \pm 0,3 \text{ mm}$. The ear canal extension terminates at the ear simulator reference plane and is connected to the pinna as shown on Figure 7b).

NOTE Occluded ear simulators differing in detail from that specified in IEC 60318-4, are in current use in some countries. If such devices are used as part of the ear simulator, their characteristics should be stated when giving results of measurements of hearing aids or other devices under test made with the head and torso simulator.

4.2.5 Materials

The manikin shall have a non-porous surface, with an acoustic impedance which is large compared to that of air, and be of a material which ensures dimensional stability.

The pinna simulator shall be made from a high-quality elastomer. It is recommended that its shore-OO hardness, measured at the surface 15 mm forward to the ear opening, is $35^\circ \pm 6^\circ$, providing that it conforms with the acoustical specifications (see 4.3). Since the mechanical properties of elastomer materials are likely to change over time, a time period shall be specified for individual pinna simulators (e.g. by means of an expiration date), over which the mechanical characteristics of the material are expected to remain in compliance with this specification.

NOTE Type of pinna simulator used for the measurement of a device should be stated together with the test result.

4.2.6 Markings

4.2.6.1 To facilitate azimuth alignment, the torso shall, at the waist, be equipped with markings indicating the direction of 0° azimuth.

4.2.6.2 If the head is removable from the torso, both shall be provided with markings to ensure correct alignment.

4.2.6.3 To assist reproducible placement of hearing aids or other devices under test in and around the pinna, the head surfaces in the immediate vicinity of the pinnae may be equipped with coordinate axis markings. The coordinate axes should be parallel to the axis of rotation (y-axis) and the manikin reference plane (x-axis) respectively, and have the ear canal entrance point (EEP) as their origin. Values on the x-axis shall be positive towards the front of the manikin, on the y-axis positive towards the vertex.

4.2.7 Tolerances

The tolerance on a point of a cross-section relative to contours in the figures shall be ± 4 mm for the torso (Figures 4a) to 4e), $\pm 2,5$ mm for the head (Figures 5a) to 5e)) and $\pm 1,5$ mm for the pinna (Figures 7a) to 7c)). These tolerances also apply for the distance between cross-sections and the reference plane of the manikin.

4.3 Acoustical characteristics of the manikin

4.3.1 Free field frequency response

Table 3 gives the manikin free field frequency response for pure tones at third octave intervals, in decibels relative to the free field sound pressure level. Values are stated for an elevation angle of 0° , and the azimuth angles 0° , 90° , 180° and 270° for the right ear. Corresponding symmetrical azimuth angles apply for the left ear.

NOTE 1 Difficulties may be experienced when measuring the manikin frequency response at azimuth angle 270° for frequencies of 4 kHz and above. This is due to a combination of reflections from the boundaries of the test enclosure, and the head shadow effect. Hence these values have been omitted in Table 3.

NOTE 2 The data in Table 3 are based on the studies by Maxwell and Burkhard [10] and by Münster-Swendsen [12]. The results of two subsequent studies on the manikin are described in [13] and [17].

4.3.2 Tolerances

Tolerances on the manikin free field frequency response are stated in Table 3. The values stated include the tolerances in the calibration of the occluded ear simulator, but not in the calibration of the free field microphone.

4.3.3 Openings

Any openings for access to the interior of the manikin other than the ears shall not affect the response of the manikin as specified in 4.3.1.

NOTE A suitable test method is given in 5.2.5.

5 Calibration

5.1 Atmospheric reference conditions

Reference ambient pressure: 101,325 kPa

Reference temperature: 23 °C

Reference relative humidity: 50 %

5.2 Calibration method

5.2.1 General

Measurement of acoustical characteristics of the manikin shall be performed with equipment conforming to the following specifications.

5.2.2 Test space and measurement equipment

The test space and sound source shall provide an approximation to plane progressive waves in free field conditions in the frequency range 100 Hz to 10 000 Hz.

These conditions are deemed to exist if the sound pressure levels measured at distances of 250 mm from the test point do not deviate from the sound pressure level at the test point by more than ± 2 dB. The measurement points for testing compliances shall include two points on the test axis, respectively towards and away from the sound source. Four further measurement points in the test plane shall be included: two in the reference plane, to the left and right as viewed from the sound source; the other two on the axis of rotation, above and below the test point.

NOTE 1 Elimination of reflections in the test space may either be achieved by suitable absorbent lining of the enclosure boundaries, by temporal gating of the measured signal (impulse response technique), or by delayed frequency filtering of the measured signal (time delay spectrometry).

NOTE 2 The permitted deviation of sound pressure level relative to that at the test point includes the inverse pressure/distance law, deviations from this inverse pressure/distance law and deviations due to source directionality.

NOTE 3 For an anechoic room, compliance cannot generally be expected unless the test point is further than 1 m from the boundaries and the sound source is at least 2 m from the boundaries.

The sound source shall only contain coaxial elements or a single diaphragm, and the ratio of the maximum frontal sound source dimension to source distance shall be less than 0,25. In order to avoid reflections the frontal area of the sound source baffle may be covered by a suitable absorbing material.

The acoustic test signal shall be a sinusoid with a frequency within ± 1 % of the nominal frequency, and with harmonic distortion less than 2 %.

The test space shall be equipped with fixtures permitting an accurate and repeatable positioning of the manikin in accordance with the selected test point.

The effective sound pressure level of extraneous background noise shall be at least 10 dB less than the sound pressure level in the frequency band of the test signal.