
**Zinc sulfide concentrates — Determination
of zinc content — Ion-exchange/EDTA
titrimetric method**

*Concentrés sulfurés de zinc — Dosage du zinc — Méthode par échange
d'ions et titrage à l'EDTA*



Contents

Page

1	Scope	1
2	Normative references	1
3	Principle	1
4	Reagents	2
5	Apparatus	3
6	Sample	3
7	Procedure	4
8	Expression of results	6
9	Precision	6
10	Test report	8

Annexes

A	Ion exchange resins and columns	9
B	Procedure for the preparation and determination of the mass of a predried test portion	11
C	Determination of cadmium by atomic absorption spectrometry .	13
D	Flowchart of the procedure for the acceptance of analytical values for test samples	15
E	Effect of potentially interfering elements	16
F	Derivation of precision equations	17
G	Bibliography	21

© ISO 1997

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from the publisher.

International Organization for Standardization
Case postale 56 • CH-1211 Genève 20 • Switzerland
Internet central@iso.ch
X.400 c=ch; a=400net; p=iso; o=isocs; s=central

Printed in Switzerland

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

International Standard ISO 12739 was prepared by Technical Committee ISO/TC 183, *Copper lead and zinc ores and concentrates*.

Annexes A to D form an integral part of this International Standard. Annexes E to G are for information only.

STANDARDSISO.COM : Click to view the full PDF of ISO 12739:1997

STANDARDSISO.COM : Click to view the full PDF of ISO 12739:1997

Zinc sulfide concentrates — Determination of zinc content — Ion-exchange/EDTA titrimetric method

1 Scope

This International Standard specifies an ion-exchange titrimetric method for the determination of the zinc content of zinc concentrates. The method is applicable to zinc sulfide concentrates with zinc content in the range from 11 % (m/m) to 62 % (m/m).

2 Normative references

The following standards contain provisions which, through reference in this text, constitute provisions of this International Standard. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this International Standard are encouraged to investigate the possibility of applying the most recent editions of the standards indicated below. Members of IEC and ISO maintain registers of currently valid International Standards.

ISO 385-1:1984, *Laboratory glassware — Burettes — Part 1: General requirements.*

ISO 648:1977, *Laboratory glassware — One-mark pipettes.*

ISO 1042:—¹⁾, *Laboratory glassware — One-mark volumetric flasks.*

ISO 3696:1987, *Water for analytical laboratory use — Specification and test methods.*

ISO 4787:1984, *Laboratory glassware — Volumetric glassware — Methods for use and testing of capacity.*

ISO 9599:1991, *Copper, lead and zinc sulfide concentrates — Determination of hygroscopic moisture in the analysis sample — Gravimetric method.*

ISO Guide 35:1989, *Certification of reference materials — General and statistical principles.*

3 Principle

The test portion of zinc concentrate is dissolved in hydrochloric, nitric and sulfuric acids. The acidity is adjusted to about 2 mol/l with respect to hydrochloric acid. Zinc is adsorbed on a strongly basic anion exchange resin. Some interfering ions are removed by elution with 2 mol/l hydrochloric acid solution. Zinc is eluted with an ammonia-ammonium chloride solution. Zinc is determined in the eluate by titration with EDTA at a pH of approximately 5,6 using xylenol orange indicator.

1) To be published. (Revision of ISO 1042:1983)

4 Reagents

During the analysis, only reagents of recognized analytical grade and water that complies with grade 2 of ISO 3696 shall be used.

4.1 Zinc, 99,99 % minimum purity, free from oxide prior to use.

The surface of the metal may be cleaned by immersing the metal in hydrochloric acid (4.3), diluted 1 + 9 for 1 min, washed well with water followed by an acetone rinse and dried in an oven at 50 °C.

4.2 Xylenol orange indicator (0,1 % m/m)

Mix 0,1 g of the sodium salt of xylenol orange with 100 g of potassium nitrate crystals by gently grinding in a ceramic mortar with a pestle. Mixing is considered complete when colour is uniform throughout.

4.3 Hydrochloric acid (ρ_{20} 1,16 g/ml to 1,19 g/ml)

4.4 Hydrochloric acid, diluted (1 + 1)

Add 500 ml of hydrochloric acid (4.3) to 500 ml of water.

4.5 Hydrochloric acid, diluted (1 + 5)

Add 100 ml of hydrochloric acid (4.3) to 500 ml of water.

4.6 Nitric acid (ρ_{20} 1,42 g/ml)

4.7 Nitric acid, diluted (1 + 1)

Add 500 ml of nitric acid (4.6) to 500 ml of water.

4.8 Sulfuric acid, diluted (1 + 1)

Add carefully and slowly, with stirring 500 ml of sulfuric acid (ρ_{20} 1,84 g/ml) to 500 ml of water.

4.9 Sulfuric acid, diluted (1 + 100)

Add 20 ml of dilute sulfuric acid (4.8) to 1 000 ml of water.

4.10 Hydrofluoric acid (ρ_{20} 1,13 g/ml to 1,15 g/ml)

4.11 Ammonia solution, diluted (7 + 100)

Add 70 ml of aqueous ammonia solution (ρ_{20} 0,89 g/ml) to 1 000 ml of water.

4.12 Ammonia-ammonium chloride solution

Dissolve 20 g of ammonium chloride in 1 l of dilute ammonia solution (4.11).

4.13 Hydrochloric acid-ascorbic acid solution

Dissolve 0,25 g of ascorbic acid in 100 ml of dilute hydrochloric acid (4.5). Prepare fresh on day of use.

4.14 Ammonium fluoride solution (50 g/l)

Dissolve 50 g of ammonium fluoride in water and dilute to 1 l.

4.15 Sodium thiosulfate solution (100 g/l)

Dissolve 100 g of sodium thiosulfate pentahydrate in water and dilute to 1 l.

4.16 Buffer solution (pH = 5,5)

Dissolve 250 g of ammonium acetate and 25 ml of concentrated acetic acid (ρ_{20} 1,05 g/ml) in water and dilute to 1 l.

4.17 Para-nitrophenol indicator solution (2 g/l)

Dissolve 0,2 g of para-nitrophenol in water and dilute to 100 ml.

4.18 EDTA standard volumetric solution (0,1 mol/l)

Dissolve 37,2 g of the di-sodium salt of ethylenediaminetetraacetic acid dihydrate (EDTA) in water and dilute to 1 l.

5 Apparatus

5.1 Class A volumetric glassware complying with ISO 385-1, ISO 648 and ISO 1042 and used in accordance with ISO 4787.

5.2 Balance, capable of being read to 0,1 mg.

5.3 Laboratory hotplate

5.4 Muffle furnace, capable of operating at 800 °C.

5.5 Platinum crucibles, of 25 ml capacity.

5.6 Ion exchange columns, with general dimensions shown in annex A.

6 Sample**6.1 Test sample**

Prepare an air-equilibrated test sample in accordance with ISO 9599.

NOTE — A test sample is not required if predried test portions are to be used (see annex B).

6.2 Test portion

Taking multiple increments, extract a test portion of 0,5 g, weighed to the nearest 0,1 mg, from the test sample in such a manner that it is representative of the contents of the dish or tray. At the same time as the test portion is weighed, weigh test portions for the determination of hygroscopic moisture in accordance with ISO 9599.

Alternatively, the method specified in annex B may be used to prepare predried test portions directly from the laboratory sample.

7 Procedure

7.1 Number of determinations

Carry out the determinations at least in duplicate, as far as possible under repeatability conditions, on each test sample.

NOTE — Repeatability conditions exist where mutually independent test results are obtained with the same method on identical test material in the same laboratory by the same operator using the same equipment within short intervals of time.

7.2 Blank test

Determine a reagent blank. It is advisable to perform duplicate blank determinations every time an analysis is carried out on a laboratory sample. The blank samples are carried through the whole procedure apart from where no laboratory sample test portion is required. The volume of EDTA titrant used is V_b .

7.3 Dissolution of test portion

Place the test portion in a 300 ml conical beaker. Add 25 ml of hydrochloric acid (4.3). Cover with a watch glass and heat beaker and contents gently for 5 min.

Add 20 ml of dilute nitric acid (4.7) and 15 ml of dilute sulfuric acid (4.8). Heat and evaporate the solution to about 5 ml. Cool and add with caution about 50 ml of water and boil the solution.

Cool the solution to room temperature and filter it into a 300 ml beaker through a medium-speed cellulose filter paper. Wash the beaker and filter paper thoroughly with dilute sulfuric acid (4.9), collecting the washings in the same beaker.

If an acid-insoluble material is present, place the filter and insoluble residue in a platinum crucible (5.5) (see note below) and gently reduce the paper to ashes in the muffle furnace (5.4) at 800 °C. Allow the crucible and residue to cool to ambient temperature. Add 2 ml of dilute sulfuric acid (4.8), 2 ml of nitric acid (4.6) and 2 ml of hydrofluoric acid (4.10) and evaporate the solution nearly to dryness. Cool and add water in small quantities to dissolve the soluble salts. Filter through a medium-speed cellulose filter paper and add the filtrate and washing solution to the initial solution obtained above as described in paragraphs 1 to 3.

Heat to evaporate the combined filtrates to a volume of 60 ml to 80 ml. Cool and add 16 ml of hydrochloric acid (4.3). Dilute to 100 ml with water.

NOTE — If the sample contains lead, damage to the platinum crucible may occur. An alternative fusion with a zirconium crucible and sodium peroxide may be preferable.

7.4 Preparation of the ion-exchange column

Examples of ion-exchange columns which are suitable for use are shown in annex A. Pack water-soaked cotton or glass wool pads into the bottom of the column to a thickness of about 5 mm. This will retain resin in the column during use.

Soak the resin overnight in distilled water to make a slurry. With the stopcock open carefully transfer the slurry into the column to form a settled bed. This resin bed is formed by about 16 ml of the swollen resin. Close the stopcock and put about a 5 mm thickness of water-soaked glass wool or cotton wool on top of the resin.

NOTE — It is essential to ensure that the resin is covered by liquid at all times because air trapped in a resin causes "channelling", i.e. uneven flow rate and poor efficiency in the ion exchanger. If air enters the resin bed, it is recommended that the column be emptied and then repacked.

Pass about 100 ml of hydrochloric acid (4.5) through the column ensuring that the resin is covered at all times. Adjust the flow rate to about 5 ml/min using the stopcock control. The resin can be rapidly regenerated at any time by passing 100 ml of water and then 100 ml of dilute hydrochloric acid (4.5) through the column ensuring that the resin is always covered with liquid.

7.5 Adsorption of zinc on ion-exchange column

Quantitatively transfer the test solution obtained in 7.3 to the ion-exchange column at a flow rate of about 5 ml/min.

Rinse the beaker with small increments of dilute hydrochloric acid (4.5) and transfer the washings to the column. A total washing volume of 100 ml should be sufficient. Continue to drain the column until the liquid is 5 mm above the top wool plug.

Pass 100 ml of hydrochloric-ascorbic acid solution (4.13) through the column in small quantities. Then pass 100 ml of dilute hydrochloric acid (4.5) through the column. Collect the eluate in a 500 ml beaker and discard.

7.6 Elution of zinc from ion-exchange column

Elute the adsorbed zinc from the column by passing 180 ml of ammonia-ammonium chloride solution (4.12) through the resin at a flow rate of less than 5 ml/min. Collect the eluate in a 500 ml beaker.

NOTE — The column should now be regenerated in preparation for the next test solution using the procedure described in 7.4.

7.7 Titration

Add 2 to 3 drops of para-nitrophenol indicator solution (4.17) to the column eluate obtained in 7.6. Add dilute hydrochloric acid (4.4) until the colour of the solution changes from yellow to colourless.

NOTE 1 A pH meter may be used to adjust the pH to a value 5,5 to 5,7 instead of using the para-nitrophenol indicator. Care should be taken to ensure that the electrodes are washed off with water before continuing the procedure.

Add successively to the solution, 20 ml of buffer solution (4.16), 3 ml of ammonium fluoride solution (4.14) and 5 ml of sodium thiosulfate solution (4.15). Add 0,5 g of xylenol orange indicator (4.2) and swirl to dissolve. Titrate with EDTA standard solution (4.18) until the colour changes from red to yellow. Record the volume, V_t , of EDTA standard solution required.

NOTE 2 If the test sample contains cadmium it will be eluted with the zinc and will be titrated during the procedure in 7.7. The cadmium concentration must be determined separately and a correction made for its presence. The method for the determination of cadmium is given in annex C. The effect of other elements commonly found in zinc concentrates is discussed in annex E.

7.8 Determination of the titration factor of the EDTA standard solution

NOTE — In order to obtain a relative accuracy of between 0,1 % and 0,2 %, it is necessary to standardize the EDTA standard solution with zinc at the same time and under the same conditions as the analysis. It is thus advisable for the calibration to follow the complete set of operating conditions set down for the analysis. Likewise to improve the repeatability of the calibration it is useful to prepare several zinc reference solutions.

The EDTA standard solution should be standardized as follows:

- Weigh into three separate 500 ml beakers between 0,055 g and 0,31 g of high purity zinc metal (4.1), to the nearest 0,000 1 g, depending on the zinc content of the test sample. Record these masses as m_1 , m_2 and m_3 .
- To each beaker add 15 ml of dilute hydrochloric acid (4.4). Heat gently to dissolve the metal, cool and add 150 ml of ammonia-ammonium chloride solution (4.12).
- Add 2 to 3 drops of para-nitrophenol indicator solution (4.17). Add dilute hydrochloric acid (4.4) until the colour changes from yellow to colourless. Alternatively a pH meter may be used as indicated in note 1 in 7.7
- Add successively 20 ml of buffer solution (4.16), 3 ml of ammonium fluoride solution (4.14) and 5 ml of sodium thiosulfate solution (4.15). Add 0,5 g of xylenol orange indicator (4.2) and swirl to dissolve. Titrate each beaker with EDTA standard solution (4.18) until the colour changes from red to yellow and record the volume as V_1 , V_2 and V_3 .

— Calculate the intermediate factor, f_{i_x} , for each beaker using the following formula:

$$f_{i_x} = m_x/V_x \quad \text{for } x = 1 \text{ to } 3 \quad \dots (1a)$$

where

f_{i_x} is the factor obtained from the titration;

m_x is the mass of zinc weighed, in grams;

V_x is the volume of EDTA standard solution, in millilitres.

If the range of values for f_{i_1} , f_{i_2} and f_{i_3} exceeds 0,000 01 g/ml then repeat the standardization.

Otherwise calculate the mean factor as follows:

$$f = \frac{f_{i_1} + f_{i_2} + f_{i_3}}{3} \quad \dots (1b)$$

8 Expression of results

The zinc content of the test portion, W_{zn} , expressed as a percentage by mass, is given by the following equation:

$$W_{zn} = \left[\frac{(V_t - V_b) \times f \times 100}{m} - 0,581c \right] \times \frac{100}{100 - H} \quad \dots (2)$$

where

V_t is the volume of EDTA standard solution (4.18), in millilitres, used to titrate the test solution;

V_b is the volume of EDTA standard solution (4.18), in millilitres, used to titrate the blank solution;

f is the zinc equivalence factor, in grams per millilitre, determined in 7.7;

m is the mass, in grams, of the test portion;

c is the cadmium concentration, expressed as a percentage by mass;

H is the hygroscopic moisture content, as a percentage of the test portion (in the case of predried test portion being used $H = 0$).

Calculate the zinc content of the test portion to the second decimal place.

9 Precision

9.1 Expression of precision

The precision of this analytical method is expressed by the following equations:

$$s_r = 0,000\,2\bar{X} + 0,054\,3 \quad \dots (3)$$

$$s_L = 0,002\,0\bar{X} + 0,052\,4 \quad \dots (4)$$

where

$\bar{X}$ is the mean content of zinc, expressed as a percentage by mass, in the sample;

s_r is the within-laboratory standard deviation, expressed as a percentage by mass;

s_L is the between-laboratories standard deviation, expressed as a percentage by mass.

See annex F.

9.2 Procedure for obtaining the final result

See annex D.

Calculate the following quantities from the duplicate results X_1 and X_2 (%) and process according to the flowchart in annex F:

$$\text{Mean of duplicates:} \quad \bar{X} = \frac{X_1 + X_2}{2} \quad \dots (5)$$

$$\text{Within-laboratory standard deviation (repeatability)} \quad s_r = 0,000\,2\bar{X} + 0,054\,3 \quad \dots (3)$$

$$\text{Repeatability limit} \quad r = 2,8\,s_r \quad \dots (6)$$

9.3 Between-laboratories precision

Between-laboratories precision is used to determine the agreement between the results reported by two (or more) laboratories. The assumption is that all laboratories have followed the same procedure.

Calculate the following quantities:

$$\text{Mean of final results:} \quad \mu_{12} = \frac{\mu_1 + \mu_2}{2} \quad \dots (7)$$

$$\text{Between-laboratories standard deviation} \quad s_L = 0,002\,0\mu_{12} + 0,052\,4 \quad \dots (8)$$

$$\text{Within-laboratory standard deviation} \quad s_r = 0,002\,0\mu_{12} + 0,054\,3 \quad \dots (9)$$

$$\text{Permissible tolerance} \quad P = 2,8\sqrt{s_L^2 + \frac{s_r^2}{2}} \quad \dots (10)$$

$$\text{Range} \quad E = |\mu_1 - \mu_2| \quad \dots (11)$$

where

μ_1 is the final result as a percentage by mass of zinc, reported by laboratory 1;

μ_2 is the final result as a percentage by mass of zinc, reported by laboratory 2.

If E is equal to or less than P , the final results are in a agreement.

9.4 Check of trueness

The trueness of the analytical method can be checked by applying it to a certified reference material (CRM). When the precision has been confirmed, the final laboratory result can be compared with the certified value, A_c . There are two possibilities as follows:

$$|\mu_c - A_c| \leq C \quad \dots (12)$$

If this condition exists the difference between the reported result and the certified value is statistically insignificant.

$$|\mu_c - A_c| > C \quad \dots (13)$$

If this condition exists the difference between the reported result and the certified value is statistically significant.

where

μ_c is the final result, as a percentage of zinc mass, of the certified reference material;

A_c is the certified value, as a percentage of zinc mass, of the certified reference material;

C is a quantity, as a percentage of zinc mass, depending on the type of certified reference material used as defined in 9.4.1.

9.4.1 Type of certified reference material (CRM) or reference material (RM)

Reference materials used for this purpose should be prepared and certified in accordance with ISO Guide 35.

9.4.1.1 Reference material certified/characterized by interlaboratory test programme

$$C = 2 \sqrt{\left[s_L^2 + \frac{s_r^2}{n} + s^2(A_c) \right]} \quad \dots (14)$$

where

$s^2(A_c)$ is the variance of the certified value;

n is the number of replicate determinations.

9.4.1.2 Reference material certified/characterized by only one laboratory

$$C = 2 \sqrt{s_L^2 + \frac{s_r^2}{n}} \quad \dots (15)$$

NOTE — It is recommended that this type of certified reference material be avoided unless the particular CRM is known to have an unbiased certified value.

10 Test report

The test report shall contain the following information:

- identification of the sample;
- reference to this International Standard, i.e. ISO 12739;
- zinc content of the sample, expressed as a percentage by mass;
- date on which the test was carried out;
- any occurrences noticed during the determination which may have had an influence on the results.

Annex A (normative)

Ion exchange resins and columns

A.1 Ion exchange resins

Use of a strongly basic anion exchange resin in the chloride form is mandatory with this method. It is also desirable that the grain size be in the range 150 µm to 300 µm and a dry mesh size specification of 50 mesh to 100 mesh. Such resins are manufactured by a large number of chemical companies. Some of the better known resins are listed below ²⁾.

A.2 Ion exchange columns

Typical columns are shown in figure A.1. Internal diameters are typically from 10 mm to 12 mm. Holding reservoirs (funnels) have a capacity of about 100 ml. Either cotton or glass wool plugs are suitable at the bottom and top of the resin beds. A thickness of 5 mm is suitable for the depth of the plugs. A flow rate of 5 ml/min is essential for the determination of zinc. Some calibration of stopcock positions may be necessary to achieve a suitable flow rate before running any determinations.

-
- 2) Bio-Rad Analytical Grade Resin AG 1-X8;
Mitsubishi Chemical Co. – “Diaion” S.A. 100;
Dow Chemical Co. – “Dowex” 1-X8;
Rohm & Haas Co. – “Amberlite” IRA 401;
Permutit – “Zerolit” FF;
Bayer “Lewatit” M 5080;
Fisher “Rexyn” 111;
Akzo Chemical Co. – “Imac” S 5-50.

This information is given for the convenience of users of this International Standard and does not constitute an endorsement by ISO of the product named. Equivalent products may be used if they can be shown to lead to the same results.

Dimensions in millimetres

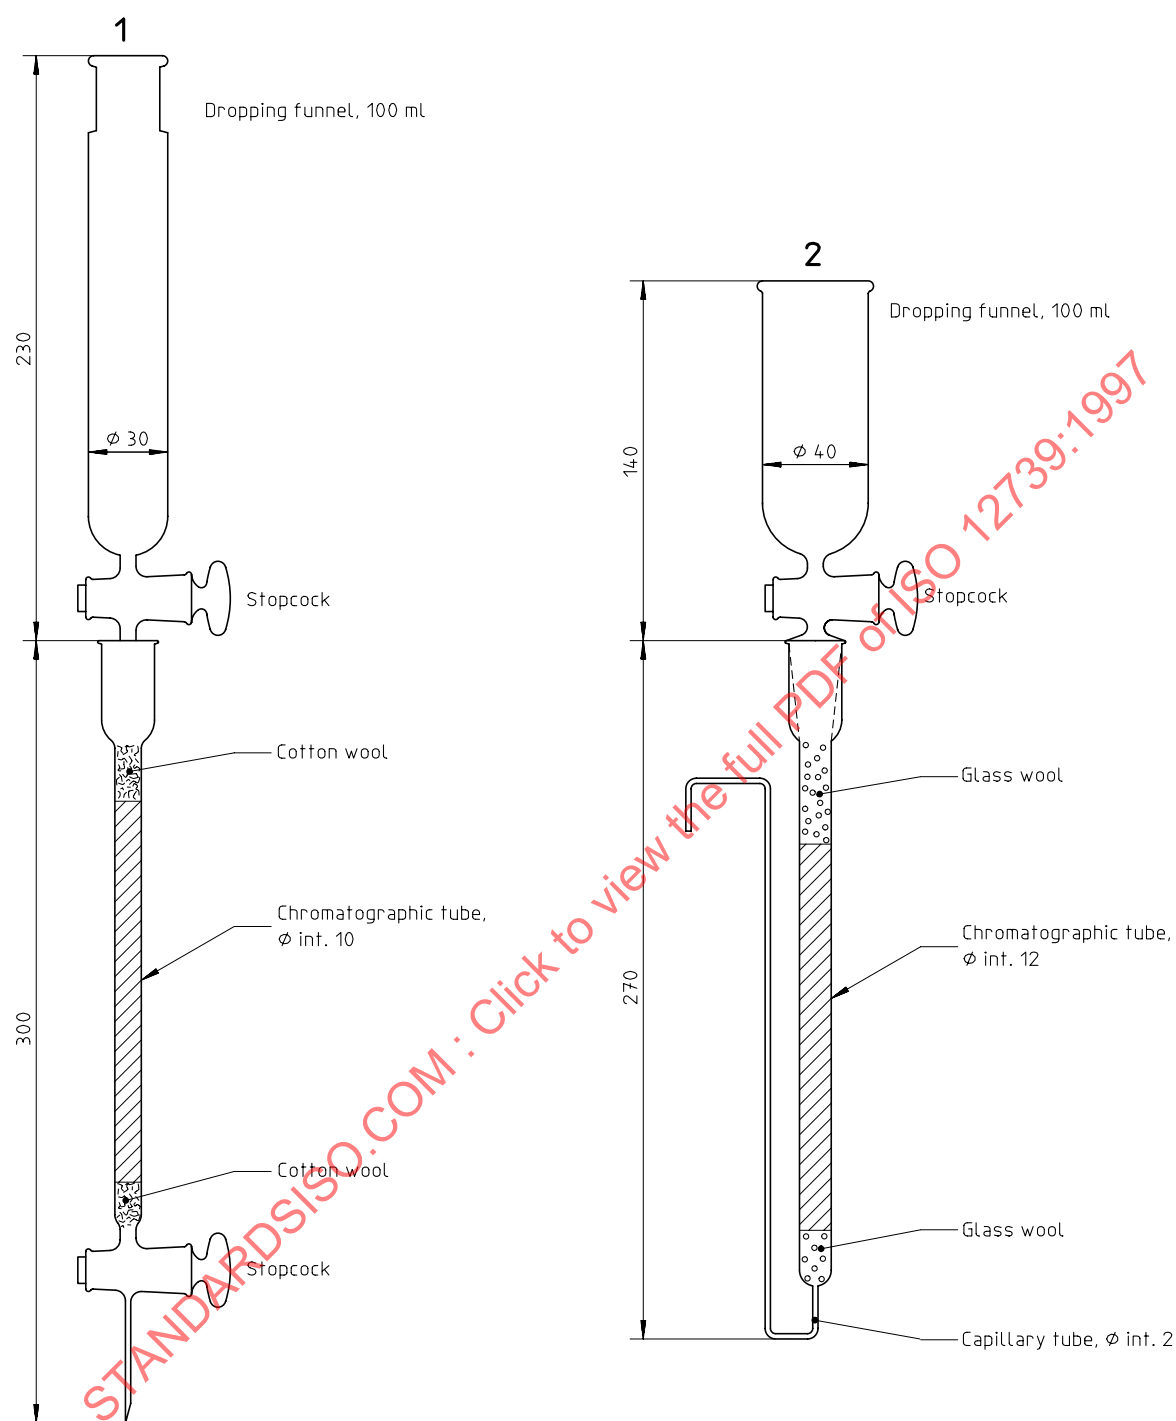


Figure A.1 — Dimensions and types of ion-exchange column

Annex B (normative)

Procedure for the preparation and determination of the mass of a predried test portion

B.1 Scope

This method is applicable to zinc sulfide concentrates not susceptible to oxidation and with hygroscopic moisture contents ranging from 0,05 % to 2 %.

B.2 Principle

The test portion to be used for analysis is dried in air in an oven maintained at $105\text{ }^{\circ}\text{C} \pm 5\text{ }^{\circ}\text{C}$. The dried test portion is then weighed and used for the analysis. No correction for moisture is required.

B.3 Reagents

B.3.1 Desiccant, such as self-indicating silica gel or anhydrous magnesium perchlorate.

WARNING — Care should be taken when disposing of exhausted magnesium perchlorate. It must be washed down the sink with a stream of running water.

B.4 Apparatus

Ordinary laboratory equipment and

B.4.1 Analytical balance, sensitive to 0,1 mg.

B.4.2 Weighing vessels, of glass, silica or corrosion-resistant metal with externally-fitting air-tight covers. For small test portions (less than 3 g) the mass of the vessel should be as small as possible, i.e. less than 20 g.

B.4.3 Laboratory oven, capable of maintaining a temperature of $105\text{ }^{\circ}\text{C} \pm 5\text{ }^{\circ}\text{C}$.

B.5 Procedure

B.5.1 Preparation of the weighing vessel

Dry the weighing vessel and vessel cover (B.4.2) by heating in a laboratory oven (B.4.3) at $105\text{ }^{\circ}\text{C} \pm 5\text{ }^{\circ}\text{C}$ for 1 h. Transfer the vessel and vessel cover to a desiccator containing suitable fresh desiccant (B.3.1) and allow to cool to ambient temperature.

B.5.2 Test portion

Weigh the dried weighing vessel and vessel cover (B.5.1). Immediately add a portion of the laboratory sample to provide a suitable predried test portion. An accurate total mass of the test portion and weighing vessel is not required at this point.

B.5.3 Determination of the test portion dry mass

Transfer the uncovered weighing vessel and test portion and vessel cover to the laboratory oven (B.4.3) and dry at $105\text{ }^{\circ}\text{C} \pm 5\text{ }^{\circ}\text{C}$ for 2 h. After the 2 h period, remove the weighing vessel and dry test portion from the oven, replace the vessel cover and allow to cool to ambient temperature in the desiccator. When cool, remove the weighing vessel and dry test portion and vessel cover from the desiccator and weigh to the nearest 0,1 mg (m_4) after slightly lifting the cover and quickly replacing it. Transfer the test portion to the appropriate analytical apparatus and immediately re-weigh the empty weighing vessel and vessel cover. Record the mass (m_5) to the nearest 0,1 mg.

NOTE — For new concentrates of unknown characteristics it is advisable to repeat the drying for another 2 h at $105\text{ }^{\circ}\text{C} \pm 5\text{ }^{\circ}\text{C}$ and to re-weigh the weighing vessel and test portion plus vessel cover to the nearest 0,1 mg (m'_4). The mass of the test portion can be considered to be constant if the difference ($m_4 - m'_4$) is less than or equal to 0,5 mg. If this condition is not achieved, the drying and weighing steps should be repeated.

B.6 Calculation of the test portion dry mass

The dry mass of the test portion m_6 , in grams, is given by the following equation:

$$m_6 = m_4 - m_5 \quad \dots \text{ (B.1)}$$

where

m_4 is the mass, in grams, of the dried test portion plus weighing vessel and its cover;

m_5 is the mass, in grams, of the empty weighing vessel plus its cover.

The mass of the dry test portion is the mass to be used to calculate the element content in the laboratory sample on a dry basis. No correction for hygroscopic moisture is required.

Annex C (normative)

Determination of cadmium by atomic absorption spectrometry

C.1 Scope

This method describes the procedure for the determination of cadmium in zinc sulfide concentrates containing cadmium in the range 0,05 % (m/m) to 0,20 % (m/m).

C.2 Principle

The sample is dissolved in hydrochloric, nitric and sulfuric acids. The mixture is evaporated to dryness and the soluble salts are taken into solution with dilute hydrochloric acid. Cadmium concentration is determined using atomic absorption spectrometry.

C.3 Reagents

C.3.1 Hydrochloric acid (ρ 1,16 g/ml to 1,19 g/ml)

C.3.2 Hydrochloric acid, diluted (1+1)

Add 500 ml of hydrochloric acid (C.3.1) to 500 ml of water.

C.3.3 Nitric acid (ρ 1,42 g/ml)

C.3.4 Nitric acid, diluted (1+1)

Add 500 ml of nitric acid (C.3.3) to 500 ml of water.

C.3.5 Sulfuric acid, diluted (1+1)

Add carefully and slowly, with stirring, 100 ml of sulfuric acid (ρ 1,84 g/ml) to 100 ml of water.

C.3.6 Standard stock solution of cadmium

Dissolve 0,5 g of high purity cadmium metal in 20 ml of dilute nitric acid (C.3.4) by heating gently. Cool and transfer to a 1 000 ml volumetric flask. Make up to the mark with water. This stock solution contains 0,5 mg of cadmium per ml of solution.

C.3.7 Cadmium standard solution

Transfer, by pipette, 10 ml of cadmium stock solution (C.3.6) to a 250 ml volumetric flask. Make up to the mark with water. Prepare on the day of use. This standard solution contains 20 μ g of cadmium per ml.

C.4 Apparatus

C.4.1 Class A volumetric glassware, complying with ISO 385-1, ISO 648 and ISO 1042 and used in accordance with ISO 4787.

C.4.2 Balance, capable of being read to 0,1 mg.

C.4.3 Hotplate

C.4.4 Atomic absorption spectrometer

C.5 Procedure

The test portion shall be 0,5 g. Weigh the test portion to the nearest 0,1 mg and place in a 200 ml beaker. Add 10 ml of hydrochloric acid (C.3.1) and 5 ml of nitric acid (C.3.3). Cover the beaker with a watch glass and boil gently. Cool and add 5 ml of sulfuric acid (C.3.5). Remove the watch glass and evaporate the solution to dryness.

Cool and add 10 ml of dilute hydrochloric acid (C.3.2) and 30 ml of water. Dissolve the soluble salts by heating gently. Filter through a medium-speed cellulose filter paper into a 100 ml volumetric flask. Wash the filter paper three times with about 10 ml of water. Allow to cool to ambient temperature and make up to volume with water. Determine the cadmium concentration by atomic absorption spectrometry.

C.6 Determination of cadmium by atomic absorption spectrometry

NOTE — The instrumental settings used for the determination of cadmium should be according to the manufacturer's recommendations. The following instructions are issued as guidelines.


The instrument should be set up with a cadmium hollow cathode lamp running at about 4 mA. The wavelength should be set to 228,8 nm with a slit width of 0,5 nm. An oxidizing acetylene-air flame is used.

The burner should be slightly rotated until a calibration solution containing 10 µg/ml of cadmium gives an absorbance reading of 0,4 absorbance units.

Three calibration solutions containing 2,00 µg, 4,00 µg and 10,00 µg of cadmium per ml should be prepared by appropriate dilution of the cadmium standard solution (C.3.7). These solutions should be used to calibrate the instrument in either the absorbance or concentration modes. The unknown solutions are then aspirated to determine the cadmium concentration of each unknown. The cadmium concentration is reported as c and is used to correct the zinc value in the calculation in clause 8.

Annex D (normative)

Flowchart of the procedure for the acceptance of analytical values for test samples

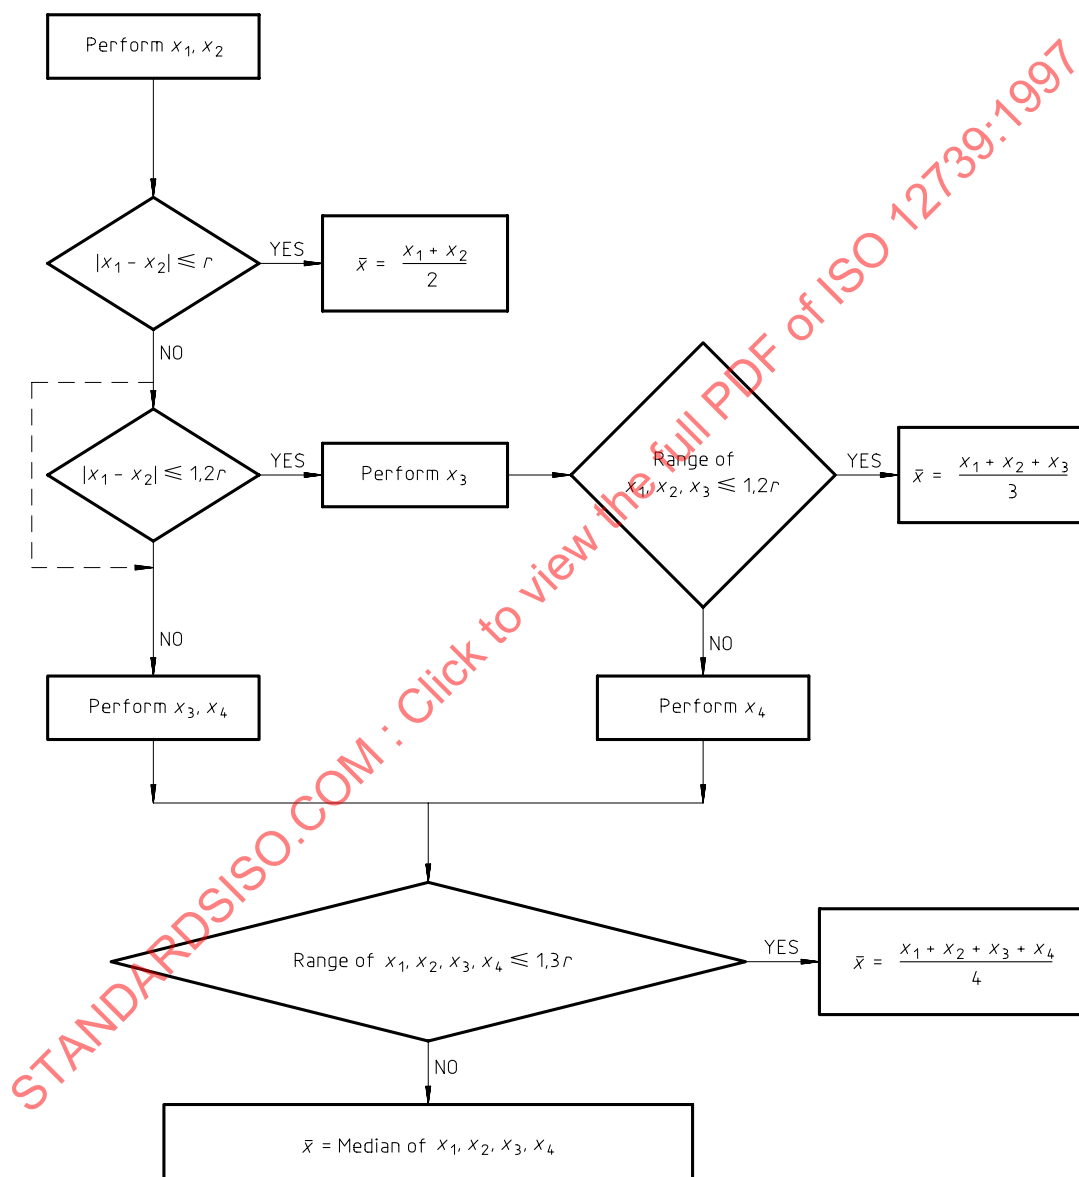

r : defined in 9.2

Annex E (informative)

Effect of potentially interfering elements

E.1 Cadmium

Cadmium is eluted at the same time as zinc. It must be determined separately and the appropriate correction must be made to the zinc concentration.

E.2 Lead

Lead is commonly present in zinc concentrates. It is largely eliminated in the filtration step given in 7.3. Small amounts of lead remaining in the filtrate are completely separated from zinc.

E.3 Iron

There is no adsorption of Fe(II) on an ion-exchange resin in 2 mol/l hydrochloric acid solution. Any Fe(III) present is reduced to Fe(II) by the hydrochloric-ascorbic acid solution.

E.4 Copper

Copper does not interfere at concentrations found in zinc concentrates.

E.5 Nickel, cobalt, manganese, calcium and aluminium

There is no adsorption of these ions on the resin from a 2 mol/l hydrochloric acid solution.