

---

---

**Clothing — Physiological effects —  
Measurement of thermal insulation by  
means of a thermal manikin**

*Vêtements — Effets physiologiques — Mesurage de l'isolation  
thermique à l'aide d'un mannequin thermique*

STANDARDSISO.COM : Click to view the full PDF of ISO 15831:2004



**PDF disclaimer**

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

STANDARDSISO.COM : Click to view the full PDF of ISO 15831:2004

© ISO 2004

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Case postale 56 • CH-1211 Geneva 20  
Tel. + 41 22 749 01 11  
Fax + 41 22 749 09 47  
E-mail [copyright@iso.org](mailto:copyright@iso.org)  
Web [www.iso.org](http://www.iso.org)

Published in Switzerland

# Contents

Page

|                                                                     |    |
|---------------------------------------------------------------------|----|
| Foreword.....                                                       | iv |
| 1 Scope.....                                                        | 1  |
| 2 Terms and definitions.....                                        | 1  |
| 3 Symbols and units .....                                           | 2  |
| 4 Principle .....                                                   | 2  |
| 5 Apparatus.....                                                    | 3  |
| 5.1 Manikin .....                                                   | 3  |
| 5.2 Controlled climatic chamber.....                                | 4  |
| 6 Selection and preparation of test garments .....                  | 5  |
| 7 Test procedure .....                                              | 5  |
| 8 Recalibration of the manikin system .....                         | 6  |
| 9 Calculation of test results .....                                 | 6  |
| 9.1 General .....                                                   | 6  |
| 9.2 Serial model — Surface area weighted thermal insulation.....    | 6  |
| 9.3 Parallel model — Surface area averaged thermal insulation ..... | 6  |
| 10 Precision of results.....                                        | 7  |
| 11 Test report.....                                                 | 7  |
| Annex A (informative) Calculation of test results .....             | 8  |
| Bibliography .....                                                  | 11 |

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 15831 was prepared by Technical Committee ISO/TC 38, *Textiles*.

STANDARDSISO.COM : Click to view the full PDF of ISO 15831:2004

# Clothing — Physiological effects — Measurement of thermal insulation by means of a thermal manikin

## 1 Scope

This International Standard describes the requirements of the thermal manikin and the test procedure used to measure the thermal insulation of a clothing ensemble, as it becomes effective for the wearer in practical use in a relatively calm environment, with the wearer either standing or moving.

NOTE This thermal insulation, among other parameters, can be used to determine the physiological effect of clothing on the wearer in specific climate/activity scenarios.

## 2 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

### 2.1

#### **clothing ensemble**

group of garments worn together on the body at the same time

### 2.2

#### **thermal insulation of clothing**

temperature difference between the wearer's skin surface and ambient atmosphere divided by the resulting dry heat flow per unit area in the direction of the temperature gradient where the dry heat flow consists of conductive, convective and radiant components

NOTE Depending on the end use of the clothing, different thermal insulation values can apply.

#### 2.2.1

##### **total thermal insulation of clothing**

$I_t$

total thermal insulation from skin to ambient atmosphere, including clothing and boundary air layer, under defined conditions measured with a stationary manikin

#### 2.2.2

##### **resultant total thermal insulation of clothing**

$I_{tr}$

total thermal insulation from skin to ambient atmosphere, including clothing and boundary air layer, under defined conditions measured with a manikin moving its legs and arms

### 3 Symbols and units

|          |                                                                                           |                                       |
|----------|-------------------------------------------------------------------------------------------|---------------------------------------|
| $a_i$    | surface area of the body segment $i$ of the manikin                                       | $\text{m}^2$                          |
| $A$      | total body surface area of the manikin                                                    | $\text{m}^2$                          |
| $f_i$    | fraction of the total manikin surface area represented by the surface area of segment $i$ |                                       |
| $H_c$    | total heating power supplied to the manikin                                               | $\text{W}$                            |
| $H_{ci}$ | heating power supplied to the body segment $i$ of the manikin                             | $\text{W}$                            |
| $I_t$    | total thermal insulation of the clothing ensemble with the manikin stationary             | $\frac{\text{m}^2\text{K}}{\text{W}}$ |
| $I_{tr}$ | resultant total thermal insulation of the clothing ensemble with the manikin moving       | $\frac{\text{m}^2\text{K}}{\text{W}}$ |
| RH       | relative humidity of the air within the climatic chamber                                  | %                                     |
| $T_a$    | air temperature within the climatic chamber                                               | $^{\circ}\text{C}$                    |
| $T_s$    | mean skin surface temperature of the manikin                                              | $^{\circ}\text{C}$                    |
| $T_{si}$ | skin surface temperature of the body segment $i$ of the manikin                           | $^{\circ}\text{C}$                    |
| $v_a$    | air speed in the climatic chamber                                                         | $\text{m/s}$                          |

### 4 Principle

The components of the clothing ensemble to be tested are placed on the manikin in the same arrangement as in practical use.

The manikin, in the shape and size of an adult human body and, for the measurement of  $I_{tr}$ , with movable legs and arms, is internally heated to a constant skin surface temperature, uniform over its body. The manikin is placed in a climatic chamber where defined air temperature and air speed can be set, and air humidity controlled.

There will be a dry heat flow from the manikin's skin surface area through the clothing into the ambient air, which is measured after steady-state conditions have been reached. From this heat flow, related to the nude manikin's body surface area, the clothing ensemble's thermal insulation can be calculated, considering the temperature difference between the manikin's skin surface and the ambient air.

The measurement is performed with the manikin stationary and/or moving its legs and arms, with a defined number of movements per minute and a defined stride length.


The insulation values obtained include the thermal insulation provided by the clothing and the adhering air layer around the body. They apply only to the particular clothing ensemble, as tested, and to the specific conditions of the test, particularly with respect to the air movement around the manikin.

## 5 Apparatus

### 5.1 Manikin

#### 5.1.1 Size and shape

The manikin, made from metal or plastic, shall be constructed to simulate the body of an adult human, i.e. it shall consist of an anatomically formed head, chest, abdomen, back, buttocks, arms, hands (preferably with fingers extended to allow gloves to be worn), legs and feet. The manikin shall consist of at least 15 body segments, each independently controlled with regard to surface temperature and monitored for heat flow. These 15 body segments shall be arranged as shown in Figure 1. If the manikin consists of more than 20 body segments, in the evaluation of the measured data, adjacent segments shall be combined using Equation (3), in order to approximate the segment arrangement shown in Figure 1.

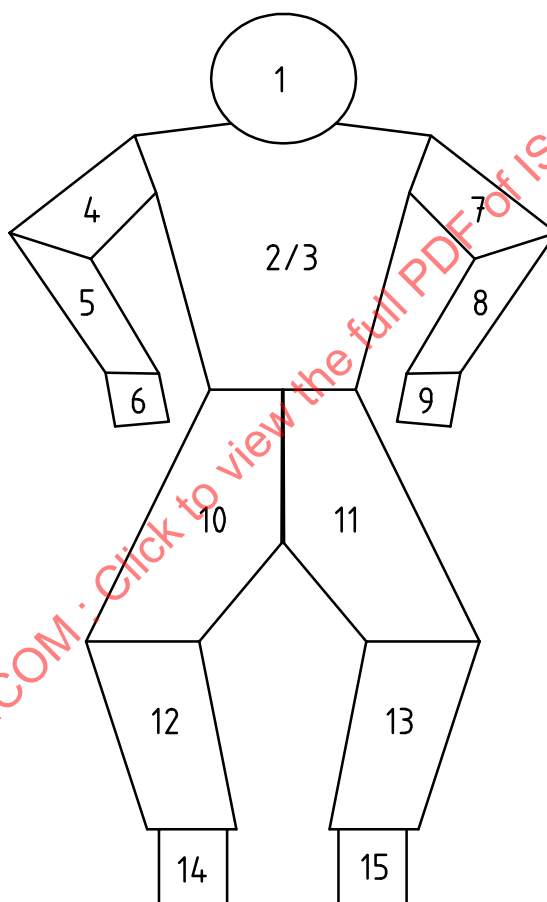

**Figure 1 — Schematic arrangement of the manikin's body segments**

The body height of the manikin shall be  $(1,70 \pm 0,15)$  m, with a body surface area of  $(1,7 \pm 0,3)$  m<sup>2</sup>.

The manikin's body proportions should correspond to those required for standard sizes of garments, because deviations in fit will affect the results.

For the measurement of  $I_t$  the manikin's arms and legs shall be movable, with joints at the shoulder, hip and knee. For the measurement of the clothing ensemble's resultant total thermal insulation,  $I_{tr}$ , the manikin, mechanically driven, shall perform  $(45 \pm 2)$  double steps per min, and  $(45 \pm 2)$  double arm movements per min cross walking. The stride length, measured from toe to toe, shall be  $(63 \pm 10)$  cm, and the length of the arm movements, measured between the wrists at the base of the thumbs,  $(53 \pm 10)$  cm.

### 5.1.2 Surface temperature

The manikin shall be constructed so as to maintain the same average constant temperature of  $(34,0 \pm 0,2) ^\circ\text{C}$  measured at all segment surfaces of its nude body.

The surface temperatures of the manikin shall be measured by at least one appropriate temperature sensor (e.g. thermocouples, thermistors, resistance temperature devices) per body segment. The sensors shall not protrude more than 0,5 mm from the manikin's surface and shall be well bonded, both mechanically and thermally, to the manikin's surface. Lead wires shall be bonded to the surface, or preferably pass through the interior of the manikin.

When calculating the mean skin surface temperature of the manikin's body, each sensor temperature shall be area-weighted, considering the portion of the body surface area covered by the sensor.

### 5.1.3 Heating equipment and power measurement

Each body segment of the manikin shall be equipped with an independently controlled heating system, whose capacity is sufficiently high to guarantee a constant surface temperature of  $(34,0 \pm 0,2) ^\circ\text{C}$  in the nude manikin at each body segment.

The dry heat flow from the manikin's body through the clothing can be determined by measuring the heating power necessary to maintain a constant surface temperature, supplied to each of the manikin's body segments during the test period.

The power measuring equipment shall be capable of giving an accurate average over the test period. Its accuracy shall be within  $\pm 2 \%$  of the value for the average power supplied to each body segment of the manikin during the test period.

## 5.2 Controlled climatic chamber

### 5.2.1 General

The manikin shall be placed in a controlled climatic chamber, at least  $2 \text{ m} \times 2 \text{ m} \times 2 \text{ m}$  (length  $\times$  width  $\times$  height). The air flow in the chamber may be horizontal or vertical.

In the chamber, spatial variations within 0,5 m of the manikin's surface shall not exceed the following:

- a) air temperature  $\pm 1,0 ^\circ\text{C}$ ;
- b) relative humidity  $\pm 10 \%$ ;
- c) air speed  $\pm 50 \%$  of the mean value;
- d) temperature of the walls, floor and ceiling shall not differ more than 1 K from the mean air temperature.

In the chamber, temporal variations during the test period shall not exceed the following:

- e) air temperature  $\pm 0,5 ^\circ\text{C}$ ;
- f) relative humidity  $\pm 10 \%$ ;
- g) air speed  $\pm 20 \%$  of the mean value for data averaged over 3 min.

### 5.2.2 Air temperature sensor(s)

To monitor the air temperature in the chamber during the test, a single sensor with an overall accuracy of  $\pm 0,15 ^\circ\text{C}$  and a time constant not exceeding 1 min may be used. However, multiple sensors are preferable.

The temperature sensor(s) shall be placed at a distance of  $(0,5 \pm 0,1)$  m from the manikin. If a single sensor is used, it shall be at least 1,0 m above the floor of the chamber. If multiple sensors are used, they shall be spaced at equal height intervals, and their readings averaged.

### 5.2.3 Relative humidity sensor

Any humidity sensing device with an accuracy of at least  $\pm 5$  % relative humidity and a repeatability of  $\pm 3$  % is acceptable. Only one location in the chamber needs to be monitored during the test to ensure that the temporal uniformity requirements mentioned in 5.2.1 are met.

### 5.2.4 Air speed sensor

For measuring the air speed in the climatic chamber an omni-directional anemometer with  $\pm 0,05$  m/s accuracy shall be used. Measurements shall be averaged for at least 3 min at locations spaced at equal height intervals  $(0,5 \pm 0,1)$  m in front of the manikin. If it is demonstrated that the air speed does not vary temporally by more than  $\pm 0,1$  m/s, then it is not necessary to monitor air speed during a test.

## 6 Selection and preparation of test garments

It is desirable to independently test three different specimens of the clothing ensemble. However, if only one specimen is available, it shall be removed and put back on the manikin between each single measurement.

The garments tested shall be an appropriate fit to the manikin.

Garments should not normally be laundered or dry cleaned prior to testing, because different procedures may affect the results. However, if garments are cleaned the cleaning shall be in accordance with the care label, and the specific care procedures applied shall be stated in the test report.

Prior to testing, the garments shall be conditioned either at  $(20 \pm 5)$  °C and  $(50 \pm 20)$  % RH or at the test climate set in the climatic chamber for at least 12 h.

## 7 Test procedure

The manikin is dressed with the clothing ensemble to be tested, with each garment arranged on the appropriate part of its body as in practical use.

For the measurement of the total thermal insulation,  $I_t$ , the manikin is kept stationary, standing with its legs straight, and the arms hanging straight at its sides.

For the measurement of the resultant total thermal insulation,  $I_{tr}$ , the legs and arms of the manikin are mechanically moved, with the frequency and stride length specified in 5.1.1.

The skin surface temperature,  $T_{si}$ , at each of the manikin's body segments, is set and, during the test period, maintained at  $(34 \pm 0,2)$  °C.

The air temperature in the climatic chamber,  $T_a$ , is set to at least 12 K below the manikin's mean skin temperature,  $T_s$ , and/or to a value ensuring a minimum heat flux of 20 W/m<sup>2</sup> at each segment of the manikin.

The relative humidity in the climatic chamber is set between 30 % and 70 %, preferably 50 %.

The air speed  $v_a$  in the climatic chamber is set to  $(0,4 \pm 0,1)$  m/s.

After starting the test, allow the system to reach steady-state conditions, i.e., the skin surface temperatures,  $T_{si}$ , of the manikin's body segments and the power input to the segments during a time period of 10 min remain constant within  $\pm 0,2$  °C and  $\pm 2$  %, respectively.

After the system has reached steady-state conditions, record the manikin's skin surface temperatures,  $T_{si}$ , the air temperature,  $T_a$ , in the climatic chamber and the power input,  $H_{ci}$ , to the manikin's body segments at least every minute during the measurement period. The average of these measurements taken over a period of at least 20 min will be sufficient to determine the clothing ensemble's thermal insulation.

At least two independent tests per clothing ensemble shall be conducted. If the difference in the results between these two tests exceeds 4 %, at least one more test shall be carried out.

The thermal insulation value(s) of the clothing ensemble given in the test report shall be the arithmetic mean of the single test results.

## 8 Recalibration of the manikin system

In order to verify that the manikin system is functioning correctly, at regular time intervals an in-house "control" clothing ensemble whose thermal insulation is known, shall be tested. If this insulation value does not lie within  $\pm 4$  %, the manikin system shall be recalibrated.

## 9 Calculation of test results

### 9.1 General

The thermal insulation of the clothing ensemble tested can be calculated either by adding the area-weighted local thermal insulation at the manikin's different body segments (serial model) or by using the total heat flow from the manikin's body (parallel model). For a given clothing ensemble the results will differ significantly between the two calculation models. The specific type of garment/s and the activity/climate conditions under which it/they is/are worn will determine which of these models is used to assess the physiological effect of the clothing ensemble on its wearer.

In application standards when physiological demands on a particular clothing ensemble are specified, it is usual for a statement to be included to direct the user as to whether the application relates to the serial or parallel model in order to obtain its appropriate thermal insulation.

The serial and parallel calculation models are defined respectively in 9.2 and 9.3. The test report shall state the model on which the insulation values are based.

### 9.2 Serial model — Surface area weighted thermal insulation

The total thermal insulation,  $I_t$ , or the resultant total thermal insulation,  $I_{tr}$ , is calculated on the test results gained with the manikin respectively either stationary or moving its legs and arms, using Equation (1).

$$I_t \text{ or } I_{tr} = \sum_i f_i \times \left[ \frac{(T_{si} - T_a) \times a_i}{H_{ci}} \right] \text{ in square metre kelvins per watt} \quad (1)$$

$$\text{where } f_i = \frac{a_i}{A} \quad (2)$$

### 9.3 Parallel model — Surface area averaged thermal insulation

The total thermal insulation,  $I_t$ , or the resultant total thermal insulation,  $I_{tr}$ , is calculated on the test results gained with the manikin respectively either stationary or moving its legs and arms, using Equation (3).

$$I_t \text{ or } I_{tr} = \frac{(T_s - T_a) \times A}{H_c} \text{ in square metre kelvins per watt} \quad (3)$$

where

$$T_s = \sum_i f_i \times T_{si} \text{ in degrees centigrade} \quad (4)$$

$$H_c = \sum_i H_{ci} \text{ in watts} \quad (5)$$

## 10 Precision of results

In a round-robin test using one clothing ensemble tested with three repetitive measurements in seven laboratories with different manikins, the following precision (coefficient of variation) of the total thermal insulation and resultant total thermal insulation, respectively, has been found:

### a) Repeatability

|                 |            |       |
|-----------------|------------|-------|
| Serial model:   | $I_t$ :    | 2,6 % |
|                 | $I_{tr}$ : | 0,8 % |
| Parallel model: | $I_t$ :    | 2,4 % |
|                 | $I_{tr}$ : | 1,9 % |

### b) Reproducibility

|                 |            |       |
|-----------------|------------|-------|
| Serial model:   | $I_t$ :    | 6,8 % |
|                 | $I_{tr}$ : | 7,9 % |
| Parallel model: | $I_t$ :    | 5,3 % |
|                 | $I_{tr}$ : | 5,9 % |

## 11 Test report

The test report shall include at least the following information.

- reference to this International Standard, i.e. ISO 15831;
- description of the test sample including washing or dry cleaning procedures, if applied;
- arrangement of the garments on the manikin (e.g. was the shirt-tail tucked in? were there any zippers, and, if so, were they closed?);
- number of test specimens per clothing ensemble and number of individual measurements on each test specimen;
- air temperature,  $T_a$ , relative humidity, RH, and air speed,  $v_a$ , in the climatic chamber during the measurement period;
- arithmetic mean of the clothing ensemble's total thermal insulation,  $I_t$ , and/or resultant total thermal insulation,  $I_{tr}$ , with reference to the calculation model (serial or parallel) on which the values are based;
- details of deviations from this International Standard;
- date of test.

## Annex A (informative)

### Calculation of test results

#### A.1 General

Usually, the thermal insulation values measured with a thermal manikin are used to assess the physiological effects of clothing. This assessment is based on different physiological models, depending on the end-use of the clothing. Partly, these models are defined in specific standards of application and use different thermal insulation values gained with the manikin, i.e. total thermal insulation or effective thermal insulation or basic thermal insulation. The latter are described in A.2, e.g. for a given clothing ensemble, the difference between the basic and effective thermal insulation can amount to up to 20 %.

#### A.2 Calculation methods

In order to measure the resultant thermal insulation of the boundary air layer,  $I_a$  or  $I_{ar}$ , conduct a test with the nude manikin, respectively in a stationary or moving condition. The nude manikin should preferably be tested at the beginning and end of each series of clothing tests to assure correct system functions.

Serial model — Surface area weighted thermal insulation

$$I_a \text{ or } I_{ar} = \sum_i f_i \left[ \frac{(T_{si} - T_a) \times a_i}{H_{ci}} \right] \quad (\text{A.1})$$

$$f_i = \frac{a_i}{A}$$

Parallel model — Surface area averaged thermal insulation

$$I_a \text{ or } I_{ar} = \frac{\left[ \left( \sum_i f_i \times T_{si} \right) - T_a \right] \times A}{\sum_i H_{ci}} \quad (\text{A.2})$$

$$f_i = \frac{a_i}{A}$$

To calculate the thermal insulation of the boundary air layer,  $I_a$  or  $I_{ar}$ , use Equation (A.1) or (A.2) on the test results obtained with the nude manikin.

To calculate the basic thermal insulation,  $I_{cl}$  or  $I_{clr}$ , use Equation (A.3).

$$I_{cl} = I_t - \frac{I_a}{f_{cl}} \quad (\text{A.3 a})$$

or

$$I_{clr} = I_{tr} - \frac{I_{ar}}{f_{cl}} \quad (\text{A.3 b})$$