



**International
Standard**

ISO 16840-12

Wheelchair seating —

Part 12:

**Envelopment and immersion
characterization of seat cushions
using a dual semispherical indenter**

AMENDMENT 1

**First edition
2021-11**

**AMENDMENT 1
2025-03**



COPYRIGHT PROTECTED DOCUMENT

© ISO 2025

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: +41 22 749 01 11
Email: copyright@iso.org
Website: www.iso.org

Published in Switzerland

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

ISO draws attention to the possibility that the implementation of this document may involve the use of (a) patent(s). ISO takes no position concerning the evidence, validity or applicability of any claimed patent rights in respect thereof. As of the date of publication of this document, ISO had not received notice of (a) patent(s) which may be required to implement this document. However, implementers are cautioned that this may not represent the latest information, which may be obtained from the patent database available at www.iso.org/patents. ISO shall not be held responsible for identifying any or all such patent rights.

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 173, *Assistive products*, Subcommittee SC 1, *Wheelchairs*.

A list of all the parts of ISO 16840 can be found on the ISO website.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

STANDARDSISO.COM : Click to view the full PDF of ISO 16840-12:2021/Amd 1:2025

Wheelchair seating —

Part 12:

Envelopment and immersion characterization of seat cushions using a dual semispherical indenter

AMENDMENT 1

7.2.4.2

Replace the title of Figure 8 with the following:

Figure 8 — Load application represented as the stepwise targeted load magnitude (y axis) and loading time (x axis) with indicated data recording times

7.3.1

Replace the text with the following:

- a) Calculate and report the average pressures during the last 10 s of the recording periods, at each elevation for $425 \text{ N} \pm 5 \text{ N}$ load and $525 \text{ N} \pm 5 \text{ N}$ load.
 - Elevation a: Average of the three trials of sensors (i.e. sensors 4 and 7 in Figure 6);
 - Elevation b: Average of the three trials of sensors (i.e. sensors 3, 5, 6, 8, 12, 13, 16, and 17 in Figure 6);
 - Elevation c: Average of the three trials of sensors (i.e. sensors 2, 9, 11, 14, 15, and 18 in Figure 6);
 - Elevation d: Average of the three trials of sensors (i.e. sensors 1 and 10 in Figure 6).
- b) Calculate and report the average pressures during the last 10 s of the recording periods for the sensors in the cleft where the indenter halves are joined (gluteal cleft) for the $425 \text{ N} \pm 5 \text{ N}$ load and $525 \text{ N} \pm 5 \text{ N}$ load.
 - Gluteal cleft: Average of the three trials of sensors (i.e. sensors 5 and 6 in Figure 6).

NOTE The pressure averages at each of the elevations provide a quick reference to a cushion's ability to redistribute forces. A cushion where reported pressure values at each elevation are similar and which also distributes load to the gluteal cleft would be considered a high-envelopment cushion.

Clause 8

Replace the text with the following:

The test report shall contain the following information for each condition tested as per 7.2:

- a) a reference to this document, i.e. ISO 16840-12:2021;
- b) the name, address of the testing institution;
- c) the accreditation status of the testing institution, if any;

- d) the date of issue of the test report;
- e) a unique test report reference;
- f) date(s) of tests;
- g) the name and address of the manufacturer of the cushion;
- h) the model, type, and nominal size that uniquely describes the test cushion, including serial and batch number and internal tracking numbers, if available;
- i) a colour photograph showing the cushion in isometric view with and without the cover (if removable);
- j) the cushion cover used;
- k) the preparation of the test cushion including environment, set up, and adjustment;
- l) the model and specifications of the pressure sensors;
- m) any deviations from the test methods of this document;
- n) a list of the equipment used, and, where relevant, statement confirming that, prior to testing, the equipment was calibrated or verified against measurement standards traceable to international or national measurement standards (where applicable), and the respective calibration dates;
- o) the results of the calculations in 7.3;
- p) disclosure of measurement uncertainty (see Annex A for guidance).

NOTE Graphs of the data can be included. Suggested formats include the following:

- 1) a line graph of the average of each of the sensors 1 to 10 (Figure 9);
- 2) a bar graph of elevations a to d (Figure 10).

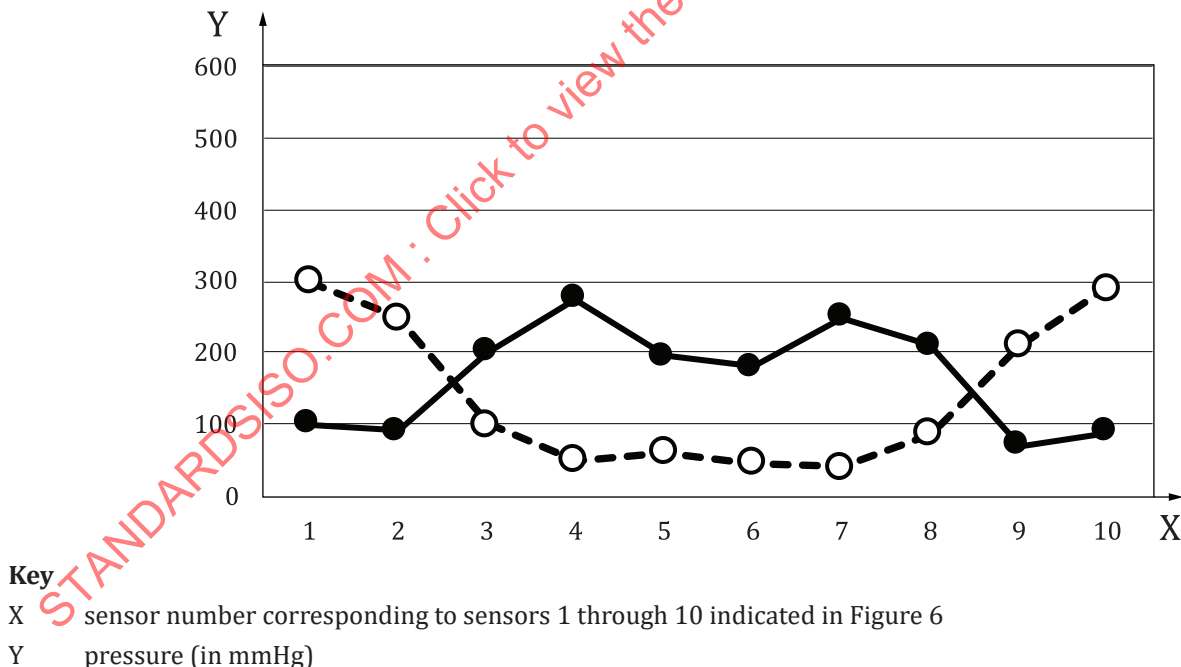


Figure 9 — Example of comparative line graph of pressure readings from the centre line of sensors for two different cushions