

INTERNATIONAL STANDARD

ISO
17937

First edition
2015-09-15

Dentistry — Osteotome

Médecine bucco-dentaire — Ostéotome

STANDARDSISO.COM : Click to view the full PDF of ISO 17937:2015



Reference number
ISO 17937:2015(E)

© ISO 2015

STANDARDSISO.COM : Click to view the full PDF of ISO 17937:2015



COPYRIGHT PROTECTED DOCUMENT

© ISO 2015, Published in Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Ch. de Blandonnet 8 • CP 401
CH-1214 Vernier, Geneva, Switzerland
Tel. +41 22 749 01 11
Fax +41 22 749 09 47
copyright@iso.org
www.iso.org

Contents

Page

Foreword	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Terms, definitions, and symbols	1
3.1 Terms and definitions	1
3.2 Symbols	2
4 Classification	2
5 Shapes	2
5.1 Sinutome	2
5.2 Condenser	3
5.3 Chisel	4
6 Material	5
6.1 Material of the working end	5
6.2 Material for the handle	5
7 Requirements	5
7.1 Dimensions	5
7.1.1 Diameter of the working end (D_1 , D_2)	5
7.1.2 Overall length	5
7.2 Marking on the working end	6
7.2.1 General	6
7.2.2 Thickness of scale line	6
7.3 Surface finish	6
7.4 Resistance to reprocessing	6
7.5 Hardness of the working end	6
7.6 Connection of shank and handle	6
8 Test method	6
8.1 Measurement of length and diameter	6
8.2 Test on surface finish	6
8.3 Test on resistance to reprocessing	6
8.4 Hardness test	6
8.5 Connection of shank	7
8.5.1 Test under tensile force	7
8.5.2 Test under torque	7
9 Marking, labelling, and instructions for use	7
9.1 Marking on the osteotome	7
9.2 Labelling on the package	7
9.3 Instructions for use	7
Bibliography	8

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT) see the following URL: [Foreword - Supplementary information](#)

The committee responsible for this document is ISO/TC 106, *Dentistry*, Subcommittee SC 4, *Dental instruments*.

Introduction

Osteotomes are instruments generally used in orthopaedic surgery. However, in dentistry, and more specific, when preparing the implant site for dental implants, certain types of osteotomes are used for bone compaction, sinus floor elevation, and jaw bone cleaving. These types of osteotomes are addressed in this International Standard.

STANDARDSISO.COM : Click to view the full PDF of ISO 17937:2015

STANDARDSISO.COM : Click to view the full PDF of ISO 17937:2015

Dentistry — Osteotome

1 Scope

This International Standard specifies requirements and their test methods for osteotomes used in dentistry for bone compaction, internal sinus floor elevation, and jaw bone cleaving. It also specifies the requirements for their marking and labelling.

2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 1942, *Dentistry — Vocabulary*

ISO 6507-1, *Metallic materials — Vickers hardness test — Part 1: Test method*

ISO 6508-1, *Metallic materials — Rockwell hardness test — Part 1: Test method*

ISO 13504, *Dentistry — General requirements for instruments and related accessories used in dental implant placement and treatment*

ISO 15087-1, *Dental elevators — Part 1: General requirements*

ISO 16443, *Dentistry — Vocabulary for dental implants systems and related procedure*

3 Terms, definitions, and symbols

3.1 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 1942, ISO 13504, ISO 16443 and the following apply.

3.1.1

osteotome

handheld dental instrument designed for bone compaction, internal sinus floor elevation, or jaw bone cleaving

Note 1 to entry: Osteotomes consist of a working tip, a shank, and a handle.

3.1.2

condenser

bone-condenser

handheld dental instrument, with conical shaped *working end* (3.1.5), used for compacting the maxillary bone surrounding the implant socket to improve the primary stability of the implant

3.1.3

chisel

handheld dental instrument designed for cleaving the jaw bone into a buccal and lingual or buccal and palatal bone lamelle in order to insert an implant in between

Note 1 to entry: Chisels can also be used selectively to remove bone for procedures such as grafting and transplantation.

3.1.4

sinutome

handheld dental instrument for performing an internal sinus floor elevation, where the sinus floor is elevated cranially through the oral cavity with different sized instruments

Note 1 to entry: Another term for internal sinus floor elevation is sinus floor elevation according to Summer.

3.1.5

working end

part of the *osteotome* (3.1.1) consisting of a *working tip* (3.1.6) and a shank connected to the *handle* (3.1.7)

3.1.6

working tip

the most frontal area of the instrument which is used for working

3.1.7

handle

area used for holding the instrument during operation

3.1.8

impact surface

backward area of the instrument used for receiving the hitting of the mallet

Note 1 to entry: Another term for mallet is hammer.

3.2 Symbols

The symbols used in [Figure 1](#) to [Figure 8](#) are the following:

- L_1 total length;
- D_1 diameter or width of the active area;
- D_2 maximum diameter at the beginning of the active area.

4 Classification

For the purposes of this International Standard, osteotomes shall be classified according to the shapes into the following types:

- Type 1: sinutome
- Type 2: condenser
- Type 3: chisel

For the purposes of this International Standard, osteotomes shall be classified according to the shape of the shanks into the following forms:

- Form A: straight shank
- Form B: offset shank

5 Shapes

5.1 Sinutome

Working tip: cylindrical

Working area: preferable as shown in detail Z, [Figure 3](#).

Dimensions in millimetres

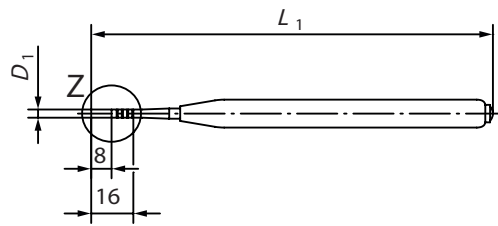


Figure 1 — Type 1, Form A: Sinutome, straight

Dimensions in millimetres


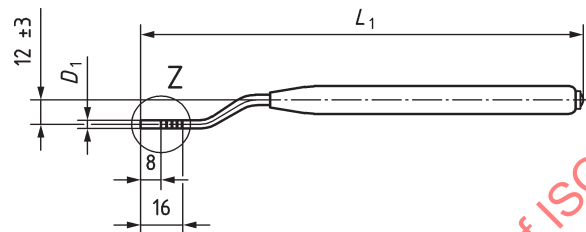


Figure 2 — Type 1, Form B: Sinutome, offset shaped



- a Plane.
- b Concave.

Figure 3 — Detail Z, working tips of sinutome

5.2 Condenser

Working tip: conical

Working area: preferable as shown in detail Z, [Figure 6](#).

Dimensions in millimetres

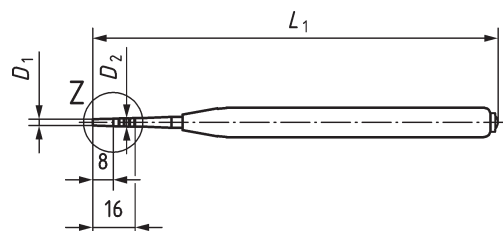


Figure 4 — Type 2, Form A: Condenser, straight

Dimensions in millimetres


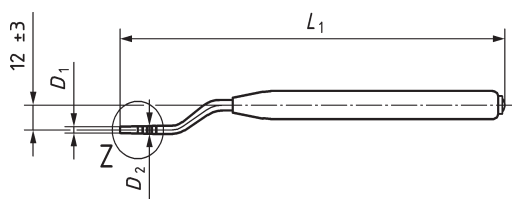


Figure 5 — Type 2, Form B: Condenser, offset



- a Convex.
- b Plane.

Figure 6 — Detail Z, working tips of condenser

5.3 Chisel

- a) Working tip: pointed, straight

Working area: preferable as shown in detail Z, [Figure 8](#).

Dimensions in millimetres


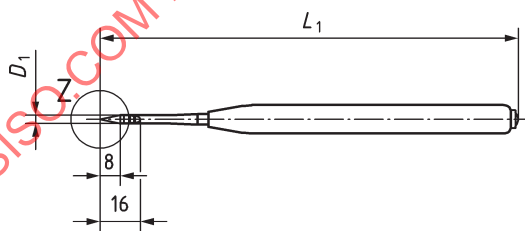


Figure 7 — Type 3, Form A: Chisel, straight with straight working tip



- a Straight with double-sided cutting edge/polished section to the point.
- b Straight with single-sided cutting edge to the tip.

Figure 8 — Detail Z, working tips of chisel

b) Working tip: pointed, curved or angled

Working area: Preferable as shown in detail Z, [Figure 10](#).

Dimensions in millimetres


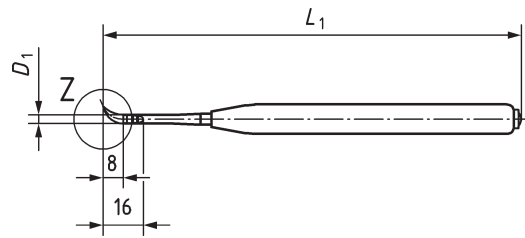


Figure 9 — Type 3, Form A: Chisel, straight with curved or angled working tip



a Curved.

b Angled.

Figure 10 — Detail Z, working tips of chisel

6 Material

6.1 Material of the working end

The materials of the working end of the osteotome shall be in accordance with ISO 13504.

6.2 Material for the handle

The material of the handle of the osteotome shall be in accordance with ISO 13504.

NOTE Some osteotomes consist of a handle with interchangeable working ends.

7 Requirements

7.1 Dimensions

7.1.1 Diameter of the working end (D_1 , D_2)

The diameter of the working end shall be within $\pm 0,1$ mm of the manufacturer's stated dimensions.

7.1.2 Overall length

The overall length of the osteotome including the handle and the working end shall not exceed 175 mm.

7.2 Marking on the working end

7.2.1 General

Marking shall be marked or carved from the tip of the working end at intervals as per the manufacturer's instructions in 2 mm steps, in order to indicate the depth of introduction of the osteotome into osseous tissue. The length from the working tip to the marking shall be within $\pm 0,1$ mm of the manufacturer's dimensions, measuring from the working tip to one of the two marking lines, whichever is nearer to the working tip, and at least the area between 8 mm and 16 mm shall be marked.

7.2.2 Thickness of scale line

The fine scale line or markings used in single dimension shall be visible without magnification.

7.3 Surface finish

The surfaces of the instruments shall be free of visible surface defects when tested in accordance with [8.2](#).

7.4 Resistance to reprocessing

There shall be no visible signs of deterioration, and the requirement for [7.5](#) and [7.6](#) shall be met when tested in accordance with [8.3](#).

7.5 Hardness of the working end

The hardness of the osteotome shall be equal or greater than 480 HV1 or 48 HRC.

7.6 Connection of shank and handle

The osteotome assembled with the shank and the handle shall not loosen when tested at the tensile force and torque as stated under [8.5.1](#) and [8.5.2](#) hereafter. Connection between impact surface and working end shall be from a material which withstands the hammering force.

8 Test method

8.1 Measurement of length and diameter

Measuring devices with the appropriate accuracy shall be used for measurements.

8.2 Test on surface finish

Normal visual inspection shall be conducted without using a magnifying glass.

8.3 Test on resistance to reprocessing

Carry out 100 reprocessing cycles in accordance with the manufacturer's instructions. The reprocessing cycle shall include the manufacturer's recommended methods of cleaning, disinfection, and sterilization. Assess visually for any signs of deterioration of the surface. Repeat the tests for hardness and connection of handle and shank.

8.4 Hardness test

Test the Vickers hardness or Rockwell hardness in accordance with ISO 6507-1 or ISO 6508-1, respectively.