
Dentistry — Shanks for rotary and oscillating instruments

*Médecine bucco-dentaire — Queues pour instruments rotatifs et
oscillants*

STANDARDSISO.COM : Click to view the full PDF of ISO 1797:2017



STANDARDSISO.COM : Click to view the full PDF of ISO 1797:2017



COPYRIGHT PROTECTED DOCUMENT

© ISO 2017, Published in Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Ch. de Blandonnet 8 • CP 401
CH-1214 Vernier, Geneva, Switzerland
Tel. +41 22 749 01 11
Fax +41 22 749 09 47
copyright@iso.org
www.iso.org

Contents

Page

Foreword	iv
1 Scope	1
2 Normative references	1
3 Terms, definitions and symbols	1
3.1 Terms and definitions	1
3.2 Symbols	2
4 Classification	3
5 Requirements	4
5.1 Dimensions	4
5.1.1 Dimensions of shanks made of metal, tungsten carbide or ceramic material	4
5.1.2 Dimensions of Type 1 plastic shanks	5
5.1.3 Shank cylindricity	6
5.1.4 Surface roughness	7
5.1.5 Location of marking	7
5.1.6 Colour code of plastic shanks	7
5.2 Material requirements	7
5.2.1 Shanks made of metal or tungsten carbide	7
5.2.2 Shanks made of ceramic materials	7
5.2.3 Shanks made of plastic materials	8
6 Sampling and pass/fail evaluation	8
7 Measurement and test methods	8
7.1 Shank diameter	8
7.2 Other dimensions	9
7.3 Shank cylindricity	9
7.4 Surface roughness	9
7.5 Vickers hardness	9
7.6 Tensile strength (only for shanks made of plastic materials)	9
7.7 Heat resistance, colour stability and stability against swelling (only for shanks made of plastic materials)	9
7.7.1 Apparatus	9
7.7.2 Procedure	9
7.7.3 Swelling resistance during reprocessing	9
Annex A (informative) Quality control	10
Bibliography	11

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT) see the following URL: www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 106, *Dentistry*, Subcommittee SC 4, *Dental instruments*.

This third edition cancels and replaces ISO 1797-1, ISO 1797-2, and ISO 1797-3, which have been technically revised with the following changes:

- a) combination of three material parts into one International Standard;
- b) reprocessing requirements for plastic shanks have been added;
- c) AQL-values have been deleted;
- d) quality control concept was moved to [Annex A](#).

Dentistry — Shanks for rotary and oscillating instruments

1 Scope

This document specifies the requirements for dimensions and material properties of shanks used in dentistry for rotary or oscillating instruments. It describes the measurement methods for the verification of the requirements.

This document is not applicable to tips fixed to the handpiece with a screw, e.g. scaler tips.

Information about the location of marking is also given. [Annex A](#) on quality control is included in order to ensure a high quality level.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 527-2, *Plastics — Determination of tensile properties — Part 2: Test conditions for moulding and extrusion plastics*

ISO 1101, *Geometrical product specifications (GPS) — Geometrical tolerancing — Tolerances of form, orientation, location and run-out*

ISO 1942, *Dentistry — Vocabulary*

ISO 3274, *Geometrical Product Specifications (GPS) — Surface texture: Profile method — Nominal characteristics of contact (stylus) instruments*

ISO 4288, *Geometrical Product Specifications (GPS) — Surface texture: Profile method — Rules and procedures for the assessment of surface texture*

ISO 6507-1, *Metallic materials — Vickers hardness test — Part 1: Test method*

ISO 8325, *Dentistry — Test methods for rotary instruments*

ISO 14457, *Dentistry — Handpieces and motors*

3 Terms, definitions and symbols

3.1 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 1942, ISO 14457 and the following apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- IEC Electropedia: available at <http://www.electropedia.org/>
- ISO Online browsing platform: available at <http://www.iso.org/obp>

3.1.1

handpiece

powered handheld device used to operate a rotary or *oscillating instrument* (3.1.3)

Note 1 to entry: This definition includes reciprocating instruments.

[SOURCE: ISO 14457:2012, 3.10, modified]


3.1.2

instrument

tool used for rotary or oscillating movements, consisting of working part, neck (if applicable) and *shank* (3.1.5), which is constructed to fit into a *handpiece* (3.1.1)

Note 1 to entry: This includes continuous rotation or *oscillating instruments* (3.1.3).

Note 2 to entry: See Figure 1.

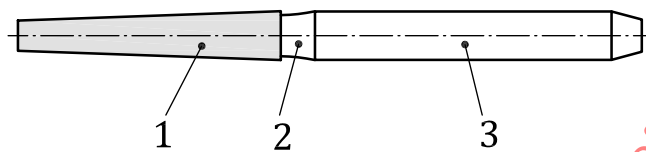

Key

- 1 working part
- 2 neck
- 3 shank

Figure 1 — Designation of instrument parts

3.1.3

oscillating instrument

instrument (3.1.2) used with an alternate (cyclic) movement, including vibrating, consisting of a *shank* (3.1.5) and a working part used in a *handpiece* (3.1.1) for dental procedures

Note 1 to entry: All movements can be combined with axial movements.

3.1.4

rotary instrument

instrument (3.1.2) used with a continuous rotation in a *handpiece* (3.1.1) consisting of a *shank* (3.1.5) and a working part used for dental procedures

3.1.5

shank

part of the shaft of a rotary or *oscillating instrument* (3.1.3) used in dentistry which is designed to fit into the chuck of a *handpiece* (3.1.1) or a handpiece for laboratory use

3.1.6

fitting length

length of the *shank* (3.1.5) that is contained within the chuck of a *handpiece* (3.1.1) or a handpiece for laboratory use

3.2 Symbols

- d_1 shank diameter
- d_2 diameter in the groove
- d_3 second distance for plastic shanks

l_1	fitting length
l_2	shoulder to end length
l_3	shoulder to groove length
l_4	width of groove
l_5	length of conical or rounded end
R_a	surface roughness
s	maximum distance from the circumference to the flat area
δ	shank cylindricity

4 Classification

Shanks for rotary or oscillating instruments are classified into the following types, according to their diameters and designs:

- Type 1: RA (right angle), CA (contra angle): diameter 2,35 mm, with groove and flat area (see [Figure 2](#));
- Type 2: HP (handpiece): diameter 2,35 mm, cylindrical (see [Figure 3](#));
- Type 3: FG (friction grip): diameter 1,6 mm, cylindrical with conical or rounded end (see [Figure 4](#));
- Type 4: HP (handpiece): diameter 3 mm cylindrical (see [Figure 3](#)).

NOTE All movements can be combined with axial movements.

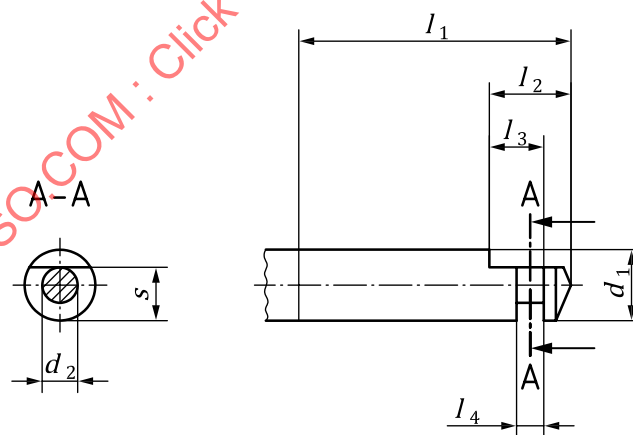


Figure 2 — Type 1 shank

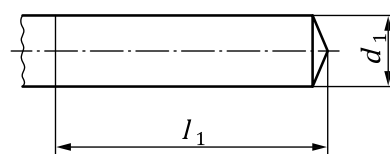


Figure 3 — Type 2 and Type 4 shank

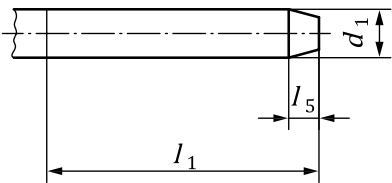


Figure 4 — Type 3 shank

5 Requirements

5.1 Dimensions

5.1.1 Dimensions of shanks made of metal, tungsten carbide or ceramic material

The dimensions and tolerances for shanks made of metal, tungsten carbide or ceramic material shall be as shown in Figure 5, Figure 6, Figure 7 and Figure 8 and as given in Table 1.

Dimensions are given in millimetres and surface roughness in micrometres.

The end of the shank for Type 1, Type 2 and Type 4 shall be flat, conical or rounded. The end of the shank for Type 3 shall be conical or rounded.

Test in accordance with 7.1 to 7.4.

Table 1 — Fitting length of shank

Dimensions in millimetres

Shank	Diameter	Fitting length, l_1 min.		
		Miniature, short	Standard, long	Extra long
Type 1 ^a	2,35	9	11	12
Type 2	2,35	15	30	30
Type 3	1,6	9	11	12
Type 4	3	—	30	30

^a The start of any enlargement on a Type 1 shank (e.g. by marking or the working head) shall be outside the fitting length.

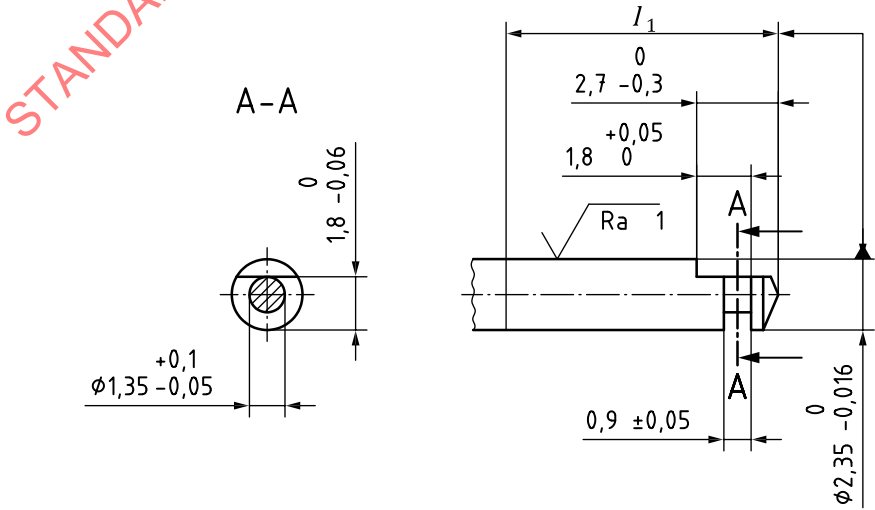


Figure 5 — Dimensions, tolerances and surface roughness for Type 1 shank

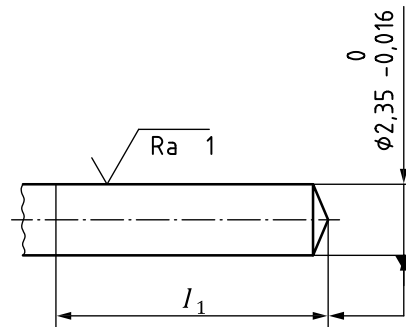


Figure 6 — Dimensions, tolerances and surface roughness for Type 2 shank

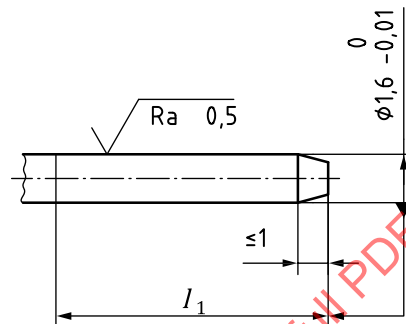


Figure 7 — Dimensions, tolerances and surface roughness for Type 3 shank

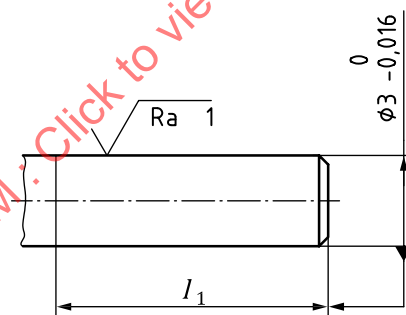


Figure 8 — Dimensions, tolerances and surface roughness for Type 4 shank

5.1.2 Dimensions of Type 1 plastic shanks

5.1.2.1 General

The dimensions and tolerances for Type 1 plastic shanks shall be as shown in [Figure 9](#) and [Figure 10](#).

Dimensions are given in millimetres and surface roughness in micrometres.

The fitting lengths shall be in accordance with [Table 1](#).

The end of the shank for Type 1 shall be flat, conical or rounded.

Test in accordance with [7.1](#) to [7.4](#), if applicable.

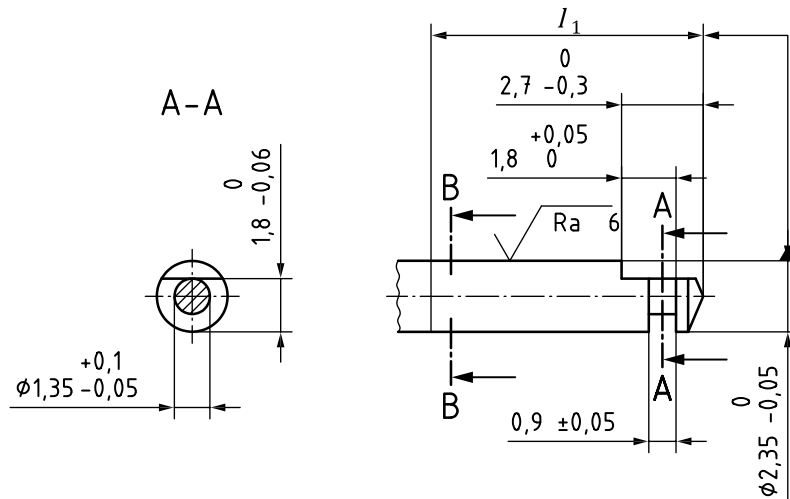


Figure 9 — Dimensions, tolerances and surface roughness for Type 1 plastic shank

5.1.2.2 Permitted shape deviations — Flattened portions of plastic shanks

Surface irregularities shall comply with the following specifications (see [Figure 10](#)).

- $d_1 = 2,35_{-0,05}^0$ mm ;
- $x = \text{max. } 0,04$ mm;
- $d_3 \leq d_1$;
- $y = \text{max. } 0,04$ mm.

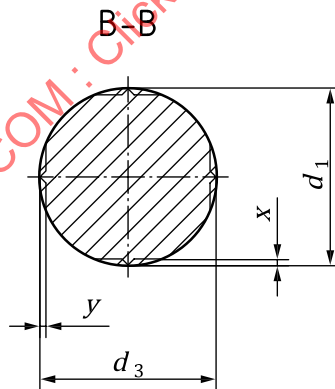


Figure 10 — Flattened portions, cross-section B-B of [Figure 9](#)

5.1.3 Shank cylindricity

The shank cylindricity for all shanks shall be within the tolerances of the acceptable shank diameter.

The definition of cylindricity is given in ISO 1101.

Test in accordance with [7.3](#).

5.1.4 Surface roughness

The surface roughness, R_a , for shanks made of metal, tungsten carbide or ceramic material, shall be for the following, as shown in [Figure 5](#) to [Figure 8](#):

- a) Type 1, Type 2, and Type 4: $\leq 1 \mu\text{m}$;
- b) Type 3: $\leq 0,5 \mu\text{m}$.

The surface roughness for polymeric materials R_a , shall be $\leq 6 \mu\text{m}$ for all types.

Test in accordance with [7.4](#).

5.1.5 Location of marking

The location of the marking, if envisaged, should be outside the fitting length.

If the marking is applied within the fitting length, l_1 , the outside diameter of the shank with the marking shall not exceed the effective diameter of the shank.

Testing shall be carried out by visual inspection.

5.1.6 Colour code of plastic shanks

The colour of the plastic shanks shall comply with the colour code of the instrument for which it is used.

Testing shall be carried out by visual inspection.

5.2 Material requirements

5.2.1 Shanks made of metal or tungsten carbide

5.2.1.1 Type of material for metal or tungsten carbide shanks

The exact type of metal or tungsten carbide material and the treatment given to it are at the discretion of the manufacturer.

5.2.1.2 Hardness for metal or tungsten carbide shanks

The hardness for shanks made of metal or tungsten carbide shall be not less than 250 HV5.

Test in accordance with [7.5](#).

5.2.2 Shanks made of ceramic materials

5.2.2.1 Type of material for ceramic shanks

The exact type of ceramic material and the treatment given to it are at the discretion of the manufacturer.

5.2.2.2 Hardness for ceramic shanks

The hardness for shanks made of ceramic material shall be not less than 1 400 HV0,5.

Test in accordance with [7.5](#).

5.2.3 Shanks made of plastic materials

5.2.3.1 Type of material for plastic shanks

The exact type of plastic material and the treatment given to it are at the discretion of the manufacturer.

5.2.3.2 Tensile test for plastic shanks

The tensile strength for shanks made of plastic shanks shall be not less than 130 MPa.

Testing shall be carried out in accordance with [7.6](#).

5.2.3.3 Heat resistance and colour stability for plastic shanks

This requirement does not apply to single use instruments.

Shanks made of plastic material shall show no signs of deformation and there shall be no recognizable colour change after testing.

Testing shall be carried out in accordance with [7.7](#).

5.2.3.4 Stability against swelling and chemicals for plastic shanks

This requirement does not apply to single use instruments.

Shanks made of plastic materials shall not swell beyond the specified tolerance range of [Figure 5](#) to [Figure 9](#) when treated with disinfecting or sterilizing solutions as recommended by the manufacturer. Shanks shall meet the tolerance range of [Figure 9](#) when sterilized according to [7.7](#).

Testing shall be carried out in accordance with [7.1](#) to [7.3](#).

5.2.3.5 Marking

Marking shall be resistant to reprocessing procedures as disinfection, cleaning and sterilization for at least five cycles according to the manufacturer's instructions, unless the instrument is marked for single use.

6 Sampling and pass/fail evaluation

Take 10 instruments at random from the validation batch and test them according to the method described in [Clause 7](#).

If eight or fewer instruments pass, the product fails.

If nine instruments pass, test 10 additional instruments. When 10 additional instruments are tested, all 10 additional instruments shall pass for the product to comply.

7 Measurement and test methods

7.1 Shank diameter

Measurements of the shank diameter shall be made in accordance with ISO 8325 with suitable measuring devices. The manufacturer shall validate that the accuracy of the measuring device is applicable.

The shank diameter, d_1 , shall be measured by traversing the length, l_1 .