

First edition  
2008-01-15

Corrected version  
2008-05-01

---

---

**Implants for surgery — Wear of total  
intervertebral spinal disc prostheses —**

**Part 1:**

**Loading and displacement parameters for  
wear testing and corresponding  
environmental conditions for test**

*Implants chirurgicaux — Usure des prothèses totales de remplacement  
des disques intervertébraux lombaires —*

*Partie 1: Paramètres de charge et de déplacement pour essais d'usure  
et conditions environnementales correspondantes*



Reference number  
ISO 18192-1:2008(E)

© ISO 2008

**PDF disclaimer**

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

STANDARDSISO.COM : Click to view the full PDF of ISO 18192-1:2008



**COPYRIGHT PROTECTED DOCUMENT**

© ISO 2008

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Case postale 56 • CH-1211 Geneva 20  
Tel. + 41 22 749 01 11  
Fax + 41 22 749 09 47  
E-mail [copyright@iso.org](mailto:copyright@iso.org)  
Web [www.iso.org](http://www.iso.org)

Published in Switzerland

# Contents

Page

|                                                                                     |           |
|-------------------------------------------------------------------------------------|-----------|
| <b>Foreword</b> .....                                                               | <b>iv</b> |
| <b>1 Scope</b> .....                                                                | <b>1</b>  |
| <b>2 Normative references</b> .....                                                 | <b>1</b>  |
| <b>3 Terms and definitions</b> .....                                                | <b>1</b>  |
| <b>4 Principle</b> .....                                                            | <b>2</b>  |
| <b>5 Reagents and materials</b> .....                                               | <b>3</b>  |
| 5.1 Fluid test medium .....                                                         | 3         |
| 5.2 Test and control specimen .....                                                 | 3         |
| <b>6 Apparatus</b> .....                                                            | <b>4</b>  |
| 6.1 Testing machine .....                                                           | 4         |
| 6.2 Means of mounting and enclosing the test specimen .....                         | 7         |
| 6.3 Means of aligning and positioning .....                                         | 7         |
| 6.4 Motion control system .....                                                     | 8         |
| 6.5 Force control system .....                                                      | 8         |
| 6.6 Lubrication system .....                                                        | 8         |
| 6.7 Temperature control system .....                                                | 8         |
| 6.8 Control station(s) .....                                                        | 8         |
| <b>7 Procedure</b> .....                                                            | <b>8</b>  |
| <b>8 Test report</b> .....                                                          | <b>9</b>  |
| <b>9 Disposal of test specimen</b> .....                                            | <b>10</b> |
| <b>Annex A (informative) Statement of rationale for test methods</b> .....          | <b>11</b> |
| <b>Annex B (informative) Load and displacement data for cervical implants</b> ..... | <b>12</b> |
| <b>Annex C (informative) Load and displacement data for lumbar implants</b> .....   | <b>13</b> |
| <b>Annex D (informative) Alternative loading conditions</b> .....                   | <b>14</b> |
| <b>Bibliography</b> .....                                                           | <b>25</b> |

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 18192-1 was prepared by Technical Committee ISO/TC 150, *Implants for surgery*, Subcommittee SC 5, *Osteosynthesis and spinal devices*.

ISO 18192 consists of the following parts, under the general title *Implants for surgery — Wear of total intervertebral spinal disc prostheses*:

- *Part 1: Loading and displacement parameters for wear testing and corresponding environmental conditions for test*

This corrected version contains corrections to the right ordinates (Z) on Figures 3 (page 6) and D.2 (page 16); a change of date to the reference in 8 a) on page 9; a revised form of the equation under Clause D.6 on page 23.

# Implants for surgery — Wear of total intervertebral spinal disc prostheses —

## Part 1:

## Loading and displacement parameters for wear testing and corresponding environmental conditions for test

### 1 Scope

This part of ISO 18192 defines a test procedure for the relative angular movement between articulating components, and specifies the pattern of the applied force, speed and duration of testing, sample configuration and test environment to be used for the wear testing of total intervertebral spinal disc prostheses.

Both lumbar and cervical prostheses are addressed. This part of ISO 18192 does not address partial disc replacements, such as nucleus replacements or facet joint replacements. The test method focuses on wear testing. Additional mechanical tests such as fatigue testing can be required.

This part of ISO 18192 does not reproduce the complex *in vivo* loads and motions. The wear data obtained with this test method will enable comparison between different types of implants but can differ from the clinical wear performance. The user of this part of ISO 18192 should consider running additional wear tests addressing specific safety issues of the individual implant design to be tested.

### 2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 14242-2, *Implants for surgery — Wear of total hip-joint prostheses — Part 2: Methods of measurement*

### 3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

#### 3.1

##### **axial rotation**

angular movement in the transverse plane around the *z*-axis

NOTE See Figure 1 c).

#### 3.2

##### **flexion/extension**

angular movement in the sagittal plane around the *y*-axis

NOTE See Figure 1 a).

### 3.3

#### **functional failure**

failure that renders the implant unable to resist the load and/or move as initially intended by the design of the implant

### 3.4

#### **lateral bending**

angular movement in the frontal plane around the  $x$ -axis

NOTE See Figure 1 b).

### 3.5

#### **mechanical failure**

onset of a defect in the material

EXAMPLE Initiation of fatigue crack.

### 3.6

#### **origin**

centre of the coordinate system located at the instantaneous centre of rotation at the neutral position of the total disc replacement

NOTE The nominal centre is specified by the design.

### 3.7

#### **user defined failure**

any failure criterion that is established and controlled by the user considering the specific design of the implant to be tested

### 3.8

#### **$x$ -axis**

positive  $x$ -axis directed anteriorly

NOTE See Figure 1.

### 3.9

#### **$y$ -axis**

positive  $y$ -axis directed laterally to the left

NOTE See Figure 1.

### 3.10

#### **$z$ -axis**

positive  $z$ -axis directed superiorly

NOTE See Figure 1.

## 4 Principle

The inferior and superior components of a test specimen are placed in position in the configuration intended for clinical use. The test apparatus transmits a specified time-varying force between the components, together with specified relative angular displacements. A load soak control specimen, if polymers are the object of investigation, is subjected to the same time-varying force to determine the creep of the test specimen and/or the amount of mass change due to fluid transfer. The test takes place in a controlled environment simulating physiological conditions.

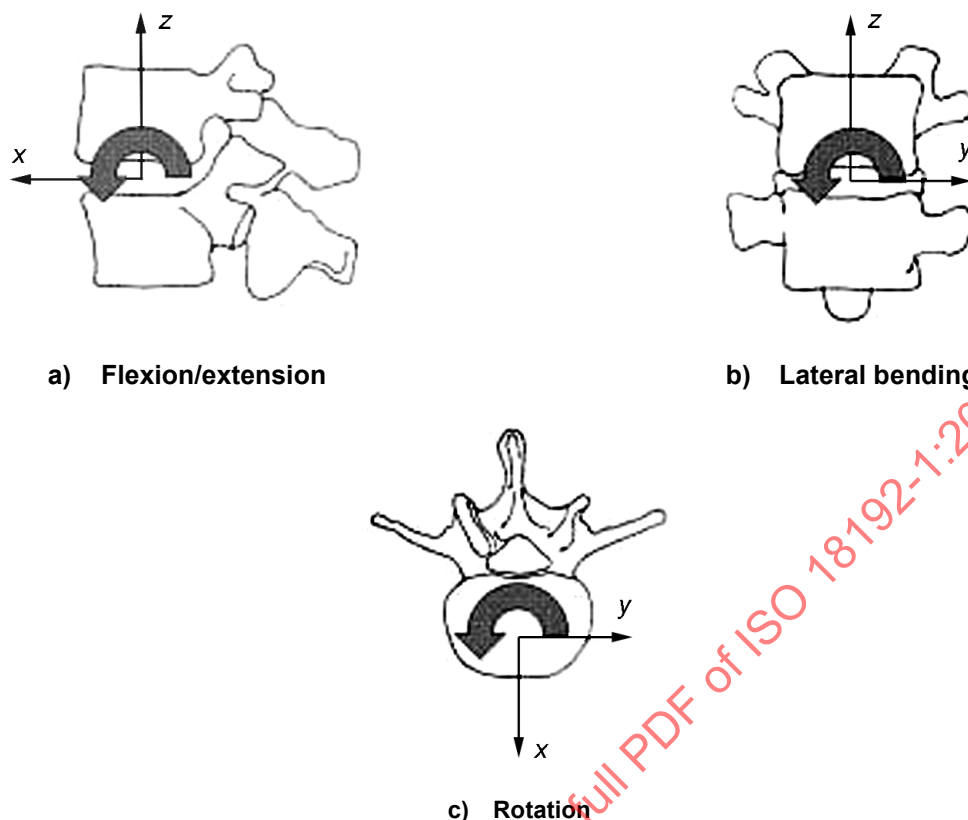


Figure 1 — Definition of the angular movements and coordinate axes

## 5 Reagents and materials

### 5.1 Fluid test medium

Calf serum diluted with de-ionized water (balance) to a concentration of  $30 \text{ g} \pm 2 \text{ g protein/l}$ .

The fluid test medium may be filtered through a  $2 \text{ }\mu\text{m}$  filter if desired.

To minimize microbial contamination, the fluid test medium should be stored frozen until required for test. An anti-microbial reagent (such as sodium azide) may be added. Such reagents can be potentially hazardous.

The addition of  $20 \text{ mmol/l}$  EDTA solution may be used to bind calcium in solution and to minimize precipitation of calcium phosphate on to the bearing surfaces. The effect of EDTA will depend on the material combination tested. The addition of EDTA shall be justified by the user.

Routine monitoring of the pH of the fluid test medium should be undertaken. If it is, the values shall be included in the test report [see 8 k) 6)].

### 5.2 Test and control specimen

Between the inferior and superior components shall be the articulating surface of the inferior and superior components, attached by its normal immediate backing (for example, bone cement or a machined replica of the inner surface of the backing) unless this is impractical due to physical features of the implant system. If the component forming the articulating surface is fixed to the backing by a rim/snap-fit system, the machined replica shall provide the same fixation conditions.

If it is not practical to use the normal backing or cement fixation, due to physical features of the implant system, the support system for the inferior and/or superior component should represent normal design

features and conditions of use but should allow removal of the component for measurement of wear without destruction.

A recommended minimum sample number of six should be used for wear testing. If less than six specimens are tested, appropriate justification shall be given.

NOTE The number of specimens tested can be the subject of national legislation.

At least one additional sample shall be used to correct weight gain by fluid uptake (load soak control). The load soak control shall be loaded according to the load profile given for the type of implant. The user may decide not to use a soak control when testing materials that do not absorb surrounding fluid (for example, metal materials).

## 6 Apparatus

**6.1 Testing machine**, capable of producing the angular displacements specified in Table 1 and Figures 2 and 3 in association with the corresponding forces specified in Table 2 and operating at a frequency of  $(1 \pm 0,1)$  Hz based on one cycle being the shortest repetitive interval for all motions and loads combined.

**Table 1 — Angular displacements of the testing machine**

|                                                                                                       | Angle | Flexion/extension | Axial rotation | Lateral bendings |
|-------------------------------------------------------------------------------------------------------|-------|-------------------|----------------|------------------|
| Cervical                                                                                              | min.  | $-7,5^\circ$      | $-4^\circ$     | $-6^\circ$       |
|                                                                                                       | max.  | $7,5^\circ$       | $4^\circ$      | $6^\circ$        |
| Lumbar                                                                                                | min.  | $-3^\circ$        | $2^\circ$      | $2^\circ$        |
|                                                                                                       | max.  | $6^\circ$         | $-2^\circ$     | $-2^\circ$       |
| NOTE The angular displacements indicated may be varied according to data given by the test requestor. |       |                   |                |                  |

**Table 2 — Load parameters of the testing machine**

|                                                                                                 | Load (N) |       |
|-------------------------------------------------------------------------------------------------|----------|-------|
| Cervical                                                                                        | max.     | 150   |
|                                                                                                 | min.     | 50    |
| Lumbar                                                                                          | max.     | 2 000 |
|                                                                                                 | min.     | 600   |
| NOTE The load parameters indicated may be varied according to data given by the test requestor. |          |       |

A defined level of shear loading shall be implemented for lumbar implants being restrained in the transverse plane. Shear loading is achieved by inclining the implant with respect to the axial load axis in the sagittal plane at the reference position (see Figure 4). Certain designs can be sensitive to shear loads. The user may intensify the test conditions by increasing the shear load and/or adding alternating load directions.

NOTE 1 The user of this document should be aware that a certain amount of shear load is generated by the motion of the device with respect to the axial load. In regard to the implant design, the user should give a justification for intended physiological conditions, especially for motion of any articulating surfaces during the load and motion cycle.

NOTE 2 See Annex A for load and motion rationale.


All angular displacement curves and load curves are smooth. The curves shall reach the given values at 0 %, 25 %, 50 % and 75 % of the motion cycle within the tolerances given in 6.4. Sample data sets are provided in Annexes B and C.

The angles are referred to moving coordinate system.

The intended sequence of the angular transformation is: lateral bending – flexion/extension – axial rotation.

NOTE 3 The sequence of the axial rotations will slightly impact the motion and the final position after each motion step (Euler angles). Due to the small angles applied, Euler sequences differing from the above will result in almost identical relative motions. The Euler sequence chosen can be selected according to the mechanical set-up of the wear testing machine.

NOTE 4 The load curve is sinusoidal.

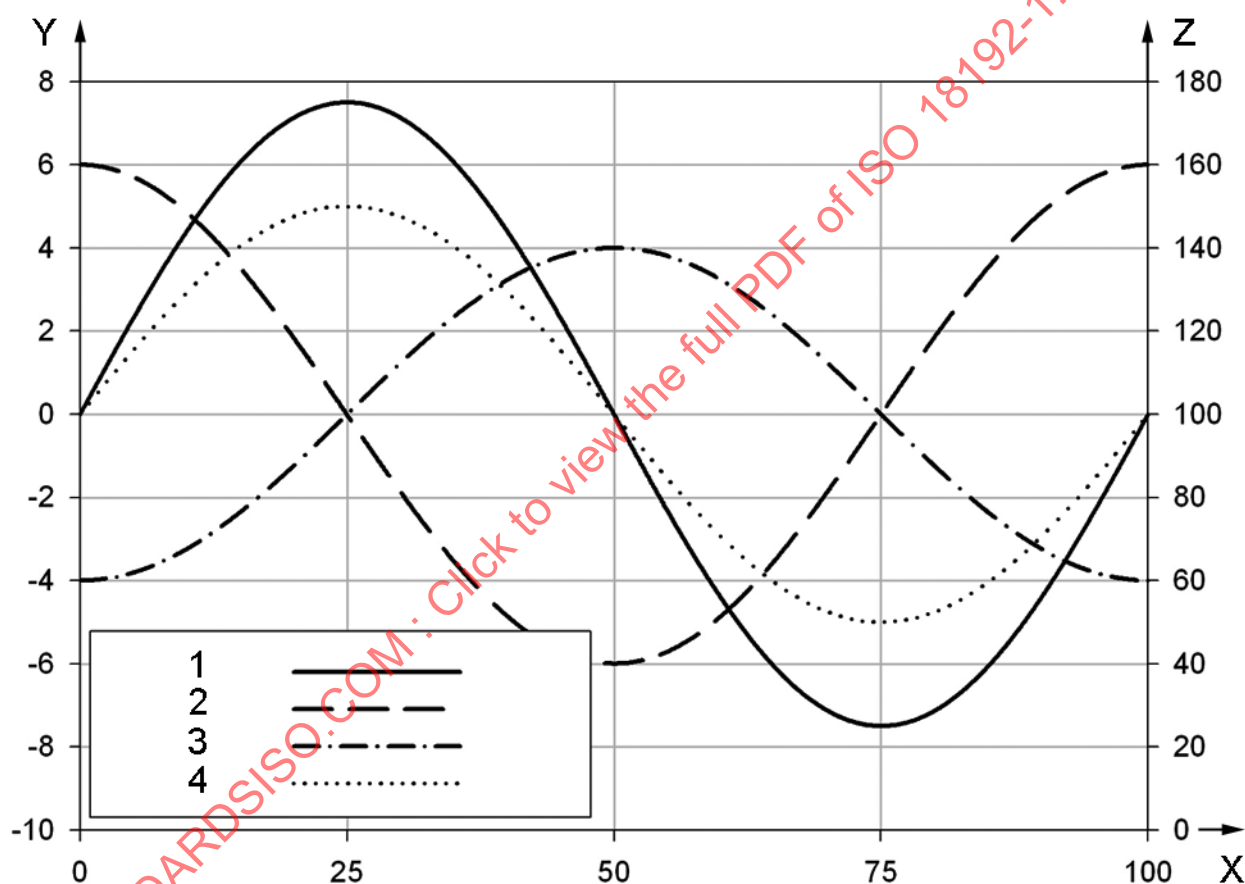


#### Key

X cycle (%)  
Y angle (°)  
Z load (N)

- 1 flexion/extension
- 2 lateral bending
- 3 rotation
- 4 load

The lateral bending is shifted 90° vs. the flexion extension axis; the axial rotation and the lateral bending are 180° out of phase.

**Figure 2 — Phasing of the displacement and load curves for cervical prostheses**

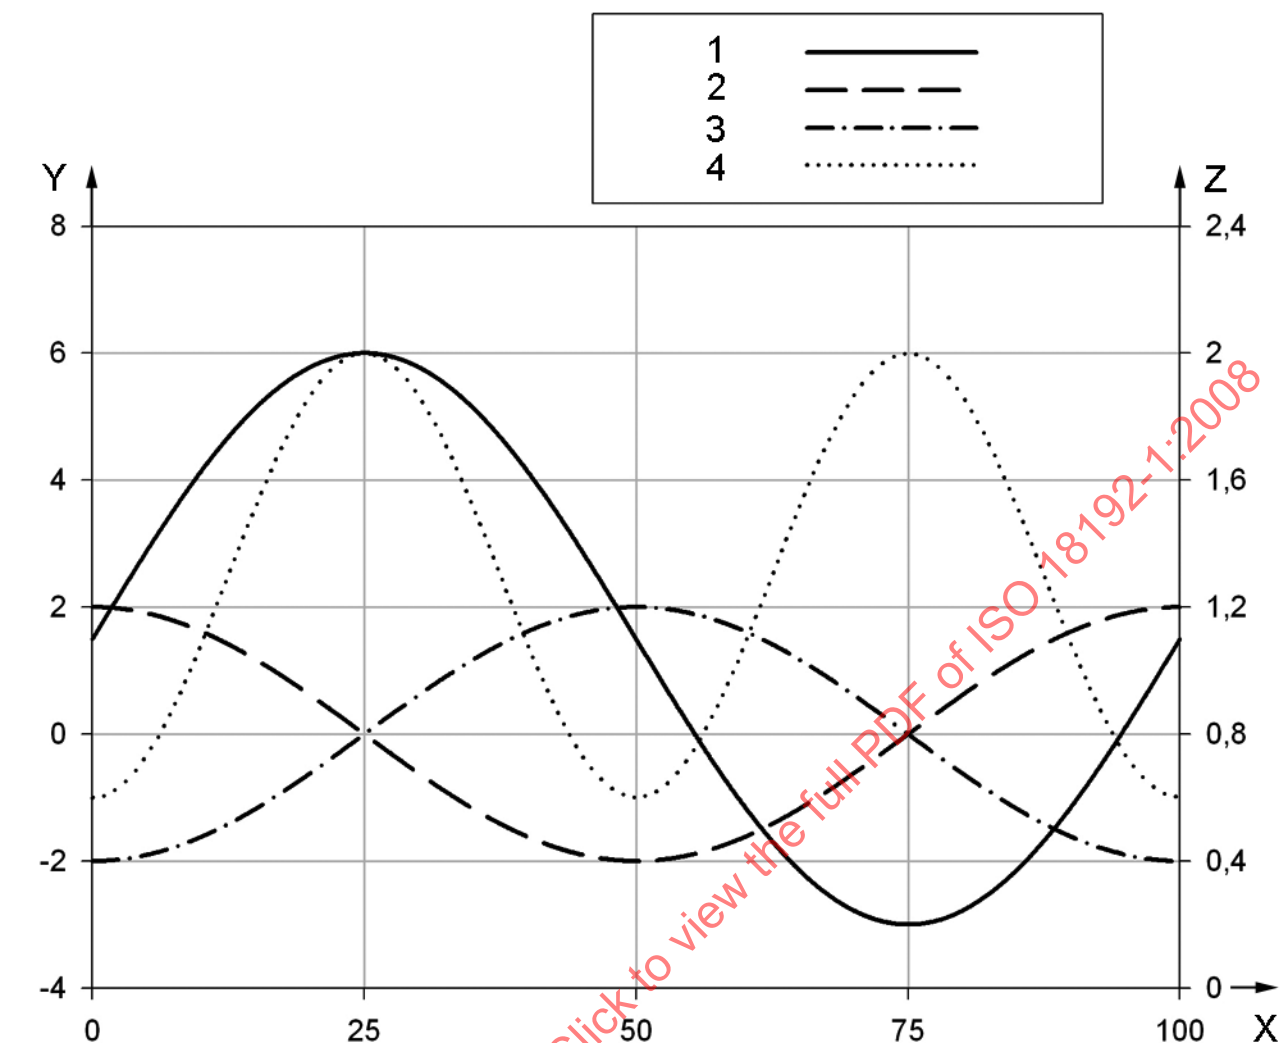**Key**

X cycle (%)

Y angle (°)

Z load (kN)

1 flexion/extension

2 lateral bending

3 rotation

4 load

The lateral bending is shifted 90° vs. the flexion extension axis; the axial rotation and the lateral bending are 180° out of phase.

**Figure 3 — Phasing of the displacement and load curves for lumbar prostheses**

**6.2 Means of mounting and enclosing the test specimen**, of a corrosion-resistant material, capable of holding inferior and superior components using attachment methods comparable to the intended anatomical fixation shall be used.


**6.3 Means of aligning and positioning**, to align the superior component of the test specimen in the superior position, so that its instantaneous axis of rotation at the neutral position is situated at the centre of the axes of rotation of the test machine and the same position and orientation can be reproduced following removal for measurement or cleaning, if required.

Align the inferior component of the test specimen, so that its instantaneous axis of rotation at the neutral position is situated at the centre of the axes of rotation of the test machine and the same position and orientation can be reproduced following removal for measurement. This alignment is intended to prevent preloads in the initial test position.

Incline the *z*-axis of lumbar implants 10° with respect to the load axis to generate enhanced shear (see Figure 4). The shear load is intended to act from posterior to anterior. Cervical implants are not inclined with respect to the axial load.

NOTE 1 Some designs using mobile bearings can generate less wear if the mobile bearing is forced by the shear load to remain in one position. In this case the user should use no inclination to generate worst case conditions.

NOTE 2 Shear forces will act on the device due to the cyclic inclination with respect to the axial load.

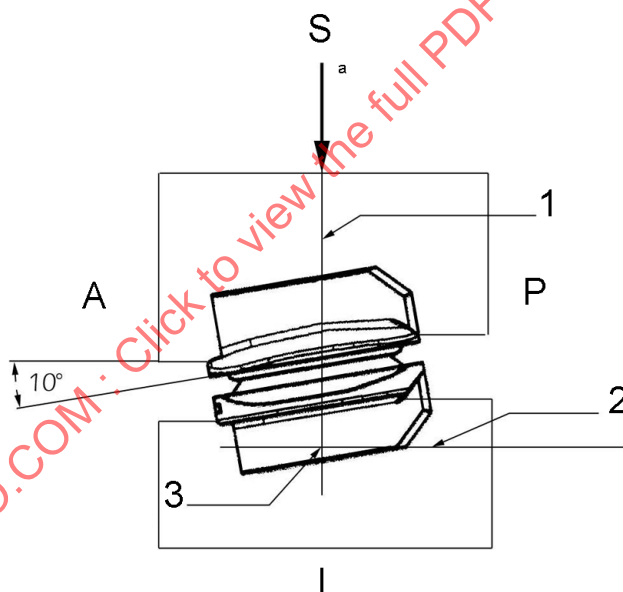

#### Key

- A anterior
- S superior
- P posterior
- I inferior
- 1 rotation axis
- 2 lateral bending axis
- 3 centre of rotation
- a axial force

**Figure 4 — Inclination of the lumbar implant in the sagittal plane to simulate shear loading**

**6.4 Motion control system**, capable of generating the angular movements of the superior component as given in Figures 2 and 3 with an accuracy of  $\pm 0,5^\circ$  at the maxima and minima of the motion and  $\pm 2\%$  of the full cycle time for phasing. For multi-station test systems, capabilities shall be assessed with all stations active.

**6.5 Force control system**, capable of generating a force in  $z$ -direction (see Figure 1) and which varies as shown in Figures 2 and 3, and capable of maintaining the magnitude of the maxima and minima of this force cycle to a tolerance of  $\pm 5\%$  of the maximum force value for the cycle and  $\pm 3\%$  of the full cycle time for phasing. For multi-station test systems, capabilities shall be assessed with all stations active.

**6.6 Lubrication system**, capable of maintaining the contact surfaces immersed in the fluid test medium.

NOTE The use of sealed enclosures can prevent evaporation and contamination.

**6.7 Temperature control system**, capable of maintaining the temperature of the fluid test medium (see 5.1) at  $(37 \pm 2)^\circ\text{C}$ .

**6.8 Control station(s)**, capable of applying the loading regime shown in Figures 2 and 3 and incorporating the requirements given in 6.2, 6.3, 6.6 and 6.7.

## 7 Procedure

**7.1** Clean the test specimen.

NOTE Cleaning of the test specimen can be carried out as described in ISO 14242-2 or by an alternative method.

**7.2** Make any initial measurements which are required to determine the subsequent amount of wear and/or creep. Calibrate all test stations with a time-varying load to ensure the system load meets the requirements in 6.5. For multi-station test systems, perform calibration with all stations active.

NOTE Methods of measurement of wear are given in ISO 14242-2.

**7.3** Mount the specimen in the testing machine.

**7.4** Take the load soak control specimen and repeat steps in 7.1, 7.2 and 7.3.

**7.5** Introduce fresh fluid test medium (see 5.1) to completely immerse the contact surfaces of the test specimen and the control specimen. Maintain the temperature of the fluid test medium at  $(37 \pm 2)^\circ\text{C}$ , taking the measurement at a location representative of the bulk temperature of the fluid. Determine the pH-value (optional).

**7.6** Wait until the specimen has reached steady state temperature.

**7.7** Start the testing machine and adjust it so that the loads and displacements specified in Figures 1 to 3 are applied to the test specimen (see 6.4 and 6.5). The curves between the defined maxima and minima in Figures 2 and 3 shall be smooth with no overshoots. Record the displacement and load waveforms at start-up, and after each change of fluid test medium for every single test station if independent test stations are used and for one test station if mechanically connected test stations are used.

**7.8** Operate the testing machine at a frequency of 1 Hz with an accuracy of  $\pm 0,1$  Hz. 1 Hz refers to one cycle per second where one cycle is defined as the shortest repetitive interval for all motions and loads combined. Test frequencies up to 2 Hz may be used. The impact of test frequencies higher than 1 Hz on the implant material behaviour as well as on the accuracy of the test machine shall be investigated by the user. Adequate justification shall be given by the user.

**7.9** Replace the fluid lost by evaporation during the test at least daily, by adding de-ionized water. Replace the fluid test medium completely at least every  $5 \times 10^5$  cycles, or every seven days, whichever is shorter.

**7.10** Stop the test for measurements at at least  $5 \times 10^5$  cycles,  $1 \times 10^6$  cycles and at least every  $1 \times 10^6$  cycles thereafter until the test is terminated (see 7.14).

**7.11** Remove the test specimen, load soak control from the testing machine and clean the test specimens.

NOTE Cleaning of the test specimen can be carried out as described in ISO 14242-2 or by an alternative method.

**7.12** Take wear measurements in accordance with ISO 14242-2.

Reinstall the test specimen and load soak control in the testing machine.

**7.13** Repeat the steps given in 7.5 to 7.12 until the test is terminated (see 7.14).

**7.14** Continue the test until one of the following occurs.

a) Completion of  $\times 10^7$  cycles (see A.5);

NOTE 1 At the request of the submitter of the specimen, the test can be continued beyond this limit.

NOTE 2 The number of cycles tested can be the subject of national legislation.

b) Functional or user defined failure of the implant;

NOTE A mechanical failure might not necessitate termination of the test since this test method attempts to characterize the time dependent wear properties of the device.

c) Failure of the testing machine to maintain the force and displacement parameters within the given tolerances (see 6.5 and 6.6).

## 8 Test report

The test report shall include the following information:

- a) reference to this part of ISO 18192, i.e. ISO 18192-1:2008;
- b) the identity of the test specimens, as stated by the submitter of the specimens for test, including size, material, type and manufacturer;
- c) a description of the testing machine, including number of stations, type of systems used for generating motions and forces, range of motions and forces, type of systems used for measuring motions and forces, arrangement for mounting specimen (see 5.2), arrangement for lubrication of articulating surfaces, arrangement for temperature control and arrangement for the exclusion of contaminant particles;
- d) the test frequency including a justification if a higher frequency than 1 Hz has been used;
- e) the inclination angle of the device and a justification of the selection in regard to the motion of the articulating surfaces;
- f) the number of specimens and a justification if less than six specimens (excluding the soak specimen) have been tested;
- g) the addition or avoidance of EDTA and a justification for doing so;
- h) the addition or avoidance of an anti-microbial reagent and a justification for doing so;
- i) the selection of the nominal centre of rotation based on the implant design;

- j) whether control specimens were used and, if not, the reference to the tests from which the control data were taken;
- k) a statement of results, including:
  - 1) total number of cycles applied;
  - 2) reason for terminating the test if less than  $\times 10^7$  cycles were applied;
  - 3) description of the surfaces of all components at which relative movement has occurred;
  - 4) description of the condition of the interfaces between subcomponents, if the components are of modular construction;
  - 5) description of the failure mode if failure occurred;
  - 6) pH values, if routine monitoring was undertaken (see 5.1);
- l) details of the method of measurement of wear and the results obtained (ISO 14242-2), namely:
  - 1) method of wear measurement (i.e. gravimetric or dimensional);
  - 2) change in mass for each measurement using the gravimetric method, or change in volume for each measurement using the dimensional method;
  - 3) both the mean wear rate (gravimetric or dimensional method) and a description of the method to determine the mean wear rate (non-linear approximation, least squares fit, etc.);
  - 4) descriptive statistics including standard deviation;
  - 5) graphic presentation of wear as a function of cycle count;
- m) any deviations made from the original test protocol including the corresponding rationale.

## 9 Disposal of test specimen

No part of the test specimen shall be used for clinical purposes after testing.

## Annex A (informative)

### Statement of rationale for test methods

**A.1** At the time of publication of this part of ISO 18192, very little knowledge about the *in vivo*, daily living loading situation of spinal disc implants is available. The aim of this test method is to give a single set of motions and loading conditions until more data becomes available.

**A.2** The choice of the test fluid has been based on current wear standards like ISO 14242-1 and ISO 14243-1. There is currently no information available indicating the composition of the fluid surrounding an artificial disc implant. The user can consider worst case scenarios for the specific implant material when selecting the appropriate test fluid.

**A.3** The magnitude of the load and motion profiles is based on range of motion data published in the literature (see e.g., Bibliography [4] to [13]). Daily living activities are assumed to cover a certain percentage of the maximum range of motion with single events of higher loads and motions. The aim of the wear test method is to simulate average loading conditions rather than the extremes. Nevertheless, the user should consider running tests at maximum loads and deflections such as migration tests, impingement tests and fatigue tests.

**A.4** The definition of shear loads has been limited to the anterior-posterior direction neglecting changes in load direction (see ISO 14630<sup>[3]</sup> and ISO 14242-1<sup>[1]</sup>). Generating the shear load by inclining the implant versus the axial load is accepted to be a simple method. The justification for doing so is to simplify the test set-up by avoiding additional force actuators. The user of this part of ISO 18192 can decide to set up a more complex load regime for implants that involve a safety risk under enhanced shear loading.

**A.5** At the time of publication of this part of ISO 18192, very little knowledge about the *in vivo* number of cycles per year is available.  $1 \times 10^7$  test cycles are assumed to incorporate a high safety factor compared to the clinical life time expected. Therefore the user of this document can decide to use a lower number of total cycles. Appropriate justification for doing so is required by this part of ISO 18192.

## Annex B (informative)

### Load and displacement data for cervical implants

| Loading cycle (%) | Flexion/extension (°) | Lateral bending (°) | Rotation (°) | Load (N) | Loading cycle (%) | Flexion/extension (°) | Lateral bending (°) | Rotation (°) | Load (N) |
|-------------------|-----------------------|---------------------|--------------|----------|-------------------|-----------------------|---------------------|--------------|----------|
| 0                 | 0,000                 | 6,000               | – 4,000      | 100,0    | 50                | 0,000                 | – 6,000             | 4,000        | 100,0    |
| 1                 | 0,471                 | 5,988               | – 3,992      | 103,1    | 51                | – 0,471               | – 5,988             | 3,992        | 96,9     |
| 2                 | 0,940                 | 5,953               | – 3,968      | 106,3    | 52                | – 0,940               | – 5,953             | 3,968        | 93,7     |
| 3                 | 1,405                 | 5,894               | – 3,929      | 109,4    | 53                | – 1,405               | – 5,894             | 3,929        | 90,6     |
| 4                 | 1,865                 | 5,811               | – 3,874      | 112,4    | 54                | – 1,865               | – 5,811             | 3,874        | 87,6     |
| 5                 | 2,318                 | 5,706               | – 3,804      | 115,5    | 55                | – 2,318               | – 5,706             | 3,804        | 84,5     |
| 6                 | 2,761                 | 5,579               | – 3,719      | 118,4    | 56                | – 2,761               | – 5,579             | 3,719        | 81,6     |
| 7                 | 3,193                 | 5,429               | – 3,619      | 121,3    | 57                | – 3,193               | – 5,429             | 3,619        | 78,7     |
| 8                 | 3,613                 | 5,258               | – 3,505      | 124,1    | 58                | – 3,613               | – 5,258             | 3,505        | 75,9     |
| 9                 | 4,019                 | 5,066               | – 3,377      | 126,8    | 59                | – 4,019               | – 5,066             | 3,377        | 73,2     |
| 10                | 4,408                 | 4,854               | – 3,236      | 129,4    | 60                | – 4,408               | – 4,854             | 3,236        | 70,6     |
| 11                | 4,781                 | 4,623               | – 3,082      | 131,9    | 61                | – 4,781               | – 4,623             | 3,082        | 68,1     |
| 12                | 5,134                 | 4,374               | – 2,916      | 134,2    | 62                | – 5,134               | – 4,374             | 2,916        | 65,8     |
| 13                | 5,467                 | 4,107               | – 2,738      | 136,4    | 63                | – 5,467               | – 4,107             | 2,738        | 63,6     |
| 14                | 5,779                 | 3,825               | – 2,550      | 138,5    | 64                | – 5,779               | – 3,825             | 2,550        | 61,5     |
| 15                | 6,068                 | 3,527               | – 2,351      | 140,5    | 65                | – 6,068               | – 3,527             | 2,351        | 59,5     |
| 16                | 6,332                 | 3,215               | – 2,143      | 142,2    | 66                | – 6,332               | – 3,215             | 2,143        | 57,8     |
| 17                | 6,572                 | 2,891               | – 1,927      | 143,8    | 67                | – 6,572               | – 2,891             | 1,927        | 56,2     |
| 18                | 6,786                 | 2,555               | – 1,703      | 145,2    | 68                | – 6,786               | – 2,555             | 1,703        | 54,8     |
| 19                | 6,973                 | 2,209               | – 1,472      | 146,5    | 69                | – 6,973               | – 2,209             | 1,472        | 53,5     |
| 20                | 7,133                 | 1,854               | – 1,236      | 147,6    | 70                | – 7,133               | – 1,854             | 1,236        | 52,4     |
| 21                | 7,264                 | 1,492               | – 0,995      | 148,4    | 71                | – 7,264               | – 1,492             | 0,995        | 51,6     |
| 22                | 7,367                 | 1,124               | – 0,750      | 149,1    | 72                | – 7,367               | – 1,124             | 0,750        | 50,9     |
| 23                | 7,441                 | 0,752               | – 0,501      | 149,6    | 73                | – 7,441               | – 0,752             | 0,501        | 50,4     |
| 24                | 7,485                 | 0,377               | – 0,251      | 149,9    | 74                | – 7,485               | – 0,377             | 0,251        | 50,1     |
| 25                | 7,500                 | 0,000               | 0,000        | 150,0    | 75                | – 7,500               | 0,000               | 0,000        | 50,0     |
| 26                | 7,485                 | – 0,377             | 0,251        | 149,9    | 76                | – 7,485               | 0,377               | – 0,251      | 50,1     |
| 27                | 7,441                 | – 0,752             | 0,501        | 149,6    | 77                | – 7,441               | 0,752               | – 0,501      | 50,4     |
| 28                | 7,367                 | – 1,124             | 0,750        | 149,1    | 78                | – 7,367               | 1,124               | – 0,750      | 50,9     |
| 29                | 7,264                 | – 1,492             | 0,995        | 148,4    | 79                | – 7,264               | 1,492               | – 0,995      | 51,6     |
| 30                | 7,133                 | – 1,854             | 1,236        | 147,6    | 80                | – 7,133               | 1,854               | – 1,236      | 52,4     |
| 31                | 6,973                 | – 2,209             | 1,472        | 146,5    | 81                | – 6,973               | 2,209               | – 1,472      | 53,5     |
| 32                | 6,786                 | – 2,555             | 1,703        | 145,2    | 82                | – 6,786               | 2,555               | – 1,703      | 54,8     |
| 33                | 6,572                 | – 2,891             | 1,927        | 143,8    | 83                | – 6,572               | 2,891               | – 1,927      | 56,2     |
| 34                | 6,332                 | – 3,215             | 2,143        | 142,2    | 84                | – 6,332               | 3,215               | – 2,143      | 57,8     |
| 35                | 6,068                 | – 3,527             | 2,351        | 140,5    | 85                | – 6,068               | 3,527               | – 2,351      | 59,5     |
| 36                | 5,779                 | – 3,825             | 2,550        | 138,5    | 86                | – 5,779               | 3,825               | – 2,550      | 61,5     |
| 37                | 5,467                 | – 4,107             | 2,738        | 136,4    | 87                | – 5,467               | 4,107               | – 2,738      | 63,6     |
| 38                | 5,134                 | – 4,374             | 2,916        | 134,2    | 88                | – 5,134               | 4,374               | – 2,916      | 65,8     |
| 39                | 4,781                 | – 4,623             | 3,082        | 131,9    | 89                | – 4,781               | 4,623               | – 3,082      | 68,1     |
| 40                | 4,408                 | – 4,854             | 3,236        | 129,4    | 90                | – 4,408               | 4,854               | – 3,236      | 70,6     |
| 41                | 4,019                 | – 5,066             | 3,377        | 126,8    | 91                | – 4,019               | 5,066               | – 3,377      | 73,2     |
| 42                | 3,613                 | – 5,258             | 3,505        | 124,1    | 92                | – 3,613               | 5,258               | – 3,505      | 75,9     |
| 43                | 3,193                 | – 5,429             | 3,619        | 121,3    | 93                | – 3,193               | 5,429               | – 3,619      | 78,7     |
| 44                | 2,761                 | – 5,579             | 3,719        | 118,4    | 94                | – 2,761               | 5,579               | – 3,719      | 81,6     |
| 45                | 2,318                 | – 5,706             | 3,804        | 115,5    | 95                | – 2,318               | 5,706               | – 3,804      | 84,5     |
| 46                | 1,865                 | – 5,811             | 3,874        | 112,4    | 96                | – 1,865               | 5,811               | – 3,874      | 87,6     |
| 47                | 1,405                 | – 5,894             | 3,929        | 109,4    | 97                | – 1,405               | 5,894               | – 3,929      | 90,6     |
| 48                | 0,940                 | – 5,953             | 3,968        | 106,3    | 98                | – 0,940               | 5,953               | – 3,968      | 93,7     |
| 49                | 0,471                 | – 5,988             | 3,992        | 103,1    | 99                | – 0,471               | 5,988               | – 3,992      | 96,9     |

NOTE 100 % loading cycle corresponds to 1 s.

## Annex C (informative)

### Load and displacement data for lumbar implants

| Loading cycle (%) | Flexion/extension (°) | Lateral bending (°) | Rotation (°) | Load (kN) | Loading cycle (%) | Flexion/extension (°) | Lateral bending (°) | Rotation (°) | Load (kN) |
|-------------------|-----------------------|---------------------|--------------|-----------|-------------------|-----------------------|---------------------|--------------|-----------|
| 0                 | 1,500                 | 2,000               | – 2,000      | 0,600     | 50                | 1,500                 | – 2,000             | 2,000        | 0,600     |
| 1                 | 1,783                 | 1,996               | – 1,996      | 0,606     | 51                | 1,217                 | – 1,996             | 1,996        | 0,606     |
| 2                 | 2,064                 | 1,984               | – 1,984      | 0,622     | 52                | 0,936                 | – 1,984             | 1,984        | 0,622     |
| 3                 | 2,343                 | 1,965               | – 1,965      | 0,649     | 53                | 0,657                 | – 1,965             | 1,965        | 0,649     |
| 4                 | 2,619                 | 1,937               | – 1,937      | 0,687     | 54                | 0,381                 | – 1,937             | 1,937        | 0,687     |
| 5                 | 2,891                 | 1,902               | – 1,902      | 0,734     | 55                | 0,109                 | – 1,902             | 1,902        | 0,734     |
| 6                 | 3,157                 | 1,860               | – 1,860      | 0,790     | 56                | – 0,157               | – 1,860             | 1,860        | 0,790     |
| 7                 | 3,416                 | 1,810               | – 1,810      | 0,854     | 57                | – 0,416               | – 1,810             | 1,810        | 0,854     |
| 8                 | 3,668                 | 1,753               | – 1,753      | 0,925     | 58                | – 0,668               | – 1,753             | 1,753        | 0,925     |
| 9                 | 3,911                 | 1,689               | – 1,689      | 1,002     | 59                | – 0,911               | – 1,689             | 1,689        | 1,002     |
| 10                | 4,145                 | 1,618               | – 1,618      | 1,084     | 60                | – 1,145               | – 1,618             | 1,618        | 1,084     |
| 11                | 4,368                 | 1,541               | – 1,541      | 1,169     | 61                | – 1,368               | – 1,541             | 1,541        | 1,169     |
| 12                | 4,580                 | 1,458               | – 1,458      | 1,256     | 62                | – 1,580               | – 1,458             | 1,458        | 1,256     |
| 13                | 4,780                 | 1,369               | – 1,369      | 1,344     | 63                | – 1,780               | – 1,369             | 1,369        | 1,344     |
| 14                | 4,967                 | 1,275               | – 1,275      | 1,431     | 64                | – 1,967               | – 1,275             | 1,275        | 1,431     |
| 15                | 5,141                 | 1,176               | – 1,176      | 1,516     | 65                | – 2,141               | – 1,176             | 1,176        | 1,516     |
| 16                | 5,299                 | 1,072               | – 1,072      | 1,598     | 66                | – 2,299               | – 1,072             | 1,072        | 1,598     |
| 17                | 5,443                 | 0,964               | – 0,964      | 1,675     | 67                | – 2,443               | – 0,964             | 0,964        | 1,675     |
| 18                | 5,572                 | 0,852               | – 0,852      | 1,746     | 68                | – 2,572               | – 0,852             | 0,852        | 1,746     |
| 19                | 5,684                 | 0,736               | – 0,736      | 1,810     | 69                | – 2,684               | – 0,736             | 0,736        | 1,810     |
| 20                | 5,780                 | 0,618               | – 0,618      | 1,866     | 70                | – 2,780               | – 0,618             | 0,618        | 1,866     |
| 21                | 5,859                 | 0,497               | – 0,497      | 1,913     | 71                | – 2,859               | – 0,497             | 0,497        | 1,913     |
| 22                | 5,920                 | 0,375               | – 0,375      | 1,951     | 72                | – 2,920               | – 0,375             | 0,375        | 1,951     |
| 23                | 5,965                 | 0,251               | – 0,251      | 1,978     | 73                | – 2,965               | – 0,251             | 0,251        | 1,978     |
| 24                | 5,991                 | 0,126               | – 0,126      | 1,994     | 74                | – 2,991               | – 0,126             | 0,126        | 1,994     |
| 25                | 6,000                 | 0,000               | 0,000        | 2,000     | 75                | – 3,000               | 0,000               | 0,000        | 2,000     |
| 26                | 5,991                 | – 0,126             | 0,126        | 1,994     | 76                | – 2,991               | 0,126               | – 0,126      | 1,994     |
| 27                | 5,965                 | – 0,251             | 0,251        | 1,978     | 77                | – 2,965               | 0,251               | – 0,251      | 1,978     |
| 28                | 5,920                 | – 0,375             | 0,375        | 1,951     | 78                | – 2,920               | 0,375               | – 0,375      | 1,951     |
| 29                | 5,859                 | – 0,497             | 0,497        | 1,913     | 79                | – 2,859               | 0,497               | – 0,497      | 1,913     |
| 30                | 5,780                 | – 0,618             | 0,618        | 1,866     | 80                | – 2,780               | 0,618               | – 0,618      | 1,866     |
| 31                | 5,684                 | – 0,736             | 0,736        | 1,810     | 81                | – 2,684               | 0,736               | – 0,736      | 1,810     |
| 32                | 5,572                 | – 0,852             | 0,852        | 1,746     | 82                | – 2,572               | 0,852               | – 0,852      | 1,746     |
| 33                | 5,443                 | – 0,964             | 0,964        | 1,675     | 83                | – 2,443               | 0,964               | – 0,964      | 1,675     |
| 34                | 5,299                 | – 1,072             | 1,072        | 1,598     | 84                | – 2,299               | 1,072               | – 1,072      | 1,598     |
| 35                | 5,141                 | – 1,176             | 1,176        | 1,516     | 85                | – 2,141               | 1,176               | – 1,176      | 1,516     |
| 36                | 4,967                 | – 1,275             | 1,275        | 1,431     | 86                | – 1,967               | 1,275               | – 1,275      | 1,431     |
| 37                | 4,780                 | – 1,369             | 1,369        | 1,344     | 87                | – 1,780               | 1,369               | – 1,369      | 1,344     |
| 38                | 4,580                 | – 1,458             | 1,458        | 1,256     | 88                | – 1,580               | 1,458               | – 1,458      | 1,256     |
| 39                | 4,368                 | – 1,541             | 1,541        | 1,169     | 89                | – 1,368               | 1,541               | – 1,541      | 1,169     |
| 40                | 4,145                 | – 1,618             | 1,618        | 1,084     | 90                | – 1,145               | 1,618               | – 1,618      | 1,084     |
| 41                | 3,911                 | – 1,689             | 1,689        | 1,002     | 91                | – 0,911               | 1,689               | – 1,689      | 1,002     |
| 42                | 3,668                 | – 1,753             | 1,753        | 0,925     | 92                | – 0,668               | 1,753               | – 1,753      | 0,925     |
| 43                | 3,416                 | – 1,810             | 1,810        | 0,854     | 93                | – 0,416               | 1,810               | – 1,810      | 0,854     |
| 44                | 3,157                 | – 1,860             | 1,860        | 0,790     | 94                | – 0,157               | 1,860               | – 1,860      | 0,790     |
| 45                | 2,891                 | – 1,902             | 1,902        | 0,734     | 95                | 0,109                 | 1,902               | – 1,902      | 0,734     |
| 46                | 2,619                 | – 1,937             | 1,937        | 0,687     | 96                | 0,381                 | 1,937               | – 1,937      | 0,687     |
| 47                | 2,343                 | – 1,965             | 1,965        | 0,649     | 97                | 0,657                 | 1,965               | – 1,965      | 0,649     |
| 48                | 2,064                 | – 1,984             | 1,984        | 0,622     | 98                | 0,936                 | 1,984               | – 1,984      | 0,622     |
| 49                | 1,783                 | – 1,996             | 1,996        | 0,606     | 99                | 1,217                 | 1,996               | – 1,996      | 0,606     |

NOTE 100 % loading cycle corresponds to 1 s.

## **Annex D** (informative)

### **Alternative loading conditions**

#### **D.1 General**

This test is not intended to replace the standard wear test as described in the main body of this document.


The user of this document can consider running an additional wear test using alternative loading conditions. A set of data is provided for this purpose. Using these data will result in three major differences compared to the regular loading conditions:

- the implant will pass the reference position (no deflection in either direction);
- there will be two stopping points within one cycle with no relative motion between the components;

NOTE The stopping points can affect the wear characteristics of certain material combinations due to breakdown of the lubrication film.

- the cervical waveform will have an increased compressive load in extension.


## D.2 Alternative loading conditions for cervical implants

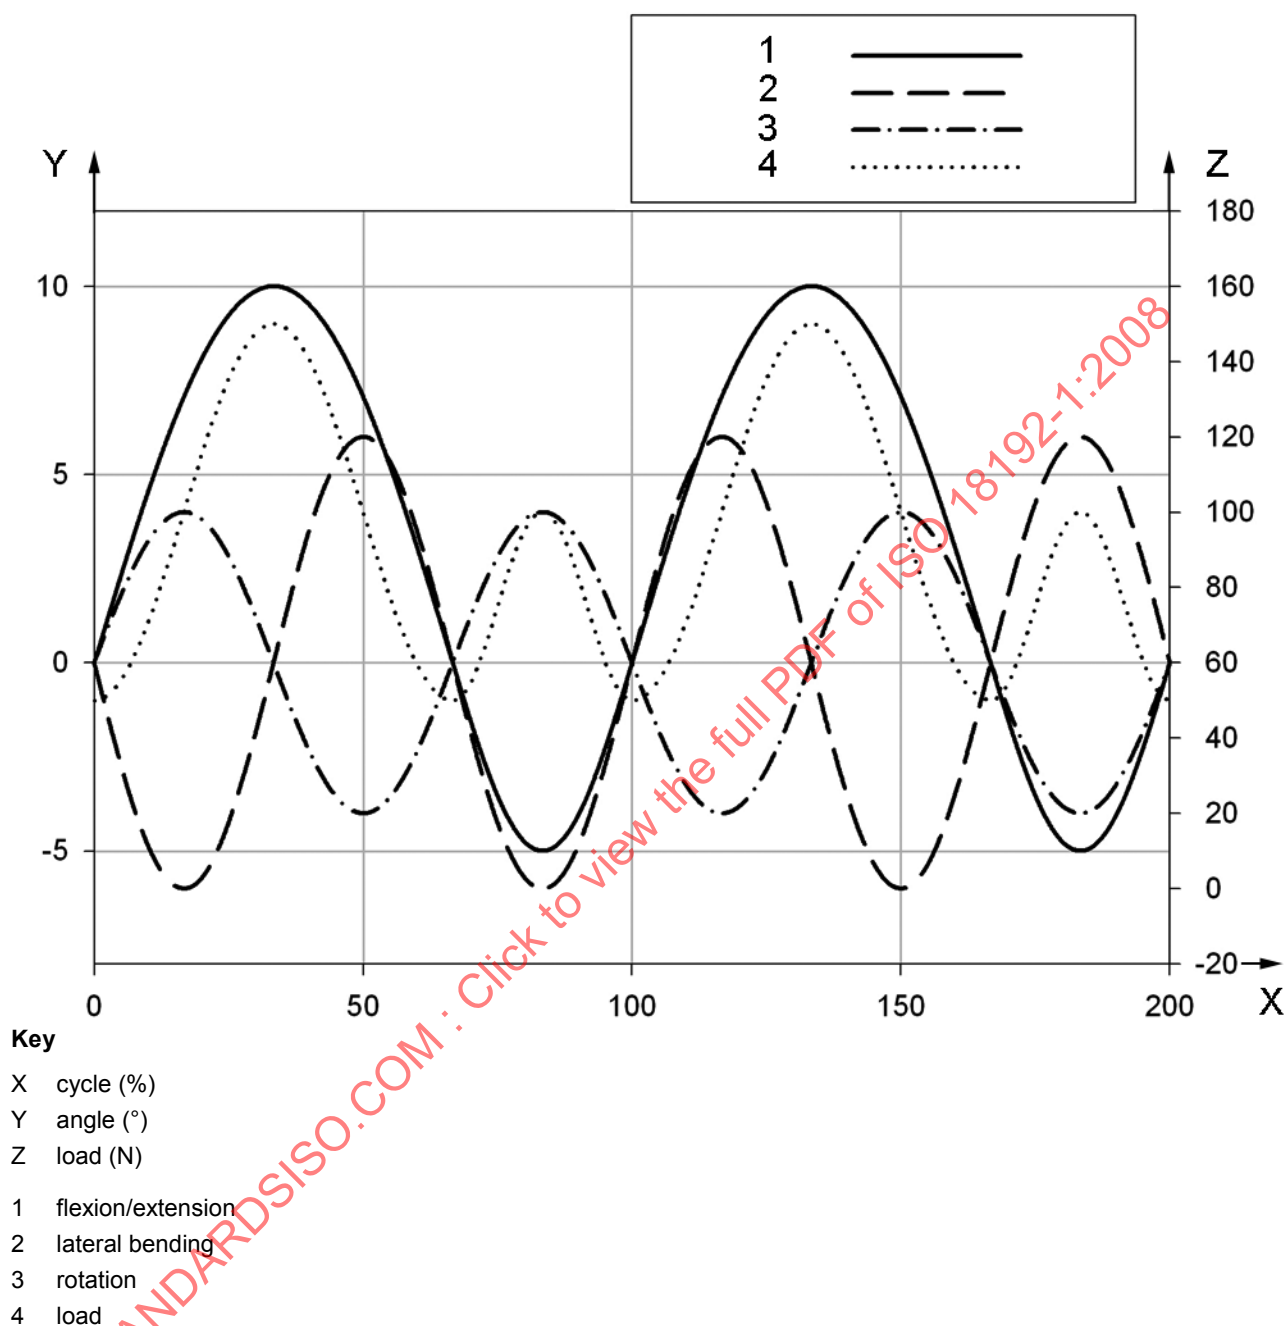

NOTE 100 % cycle corresponds to one cycle. The description of cycle given in 6.1 does not apply to Figure D.1.

Figure D.1 — Phasing of the displacement and load curves (alternative) for cervical prostheses

### D.3 Alternative loading conditions for lumbar implants

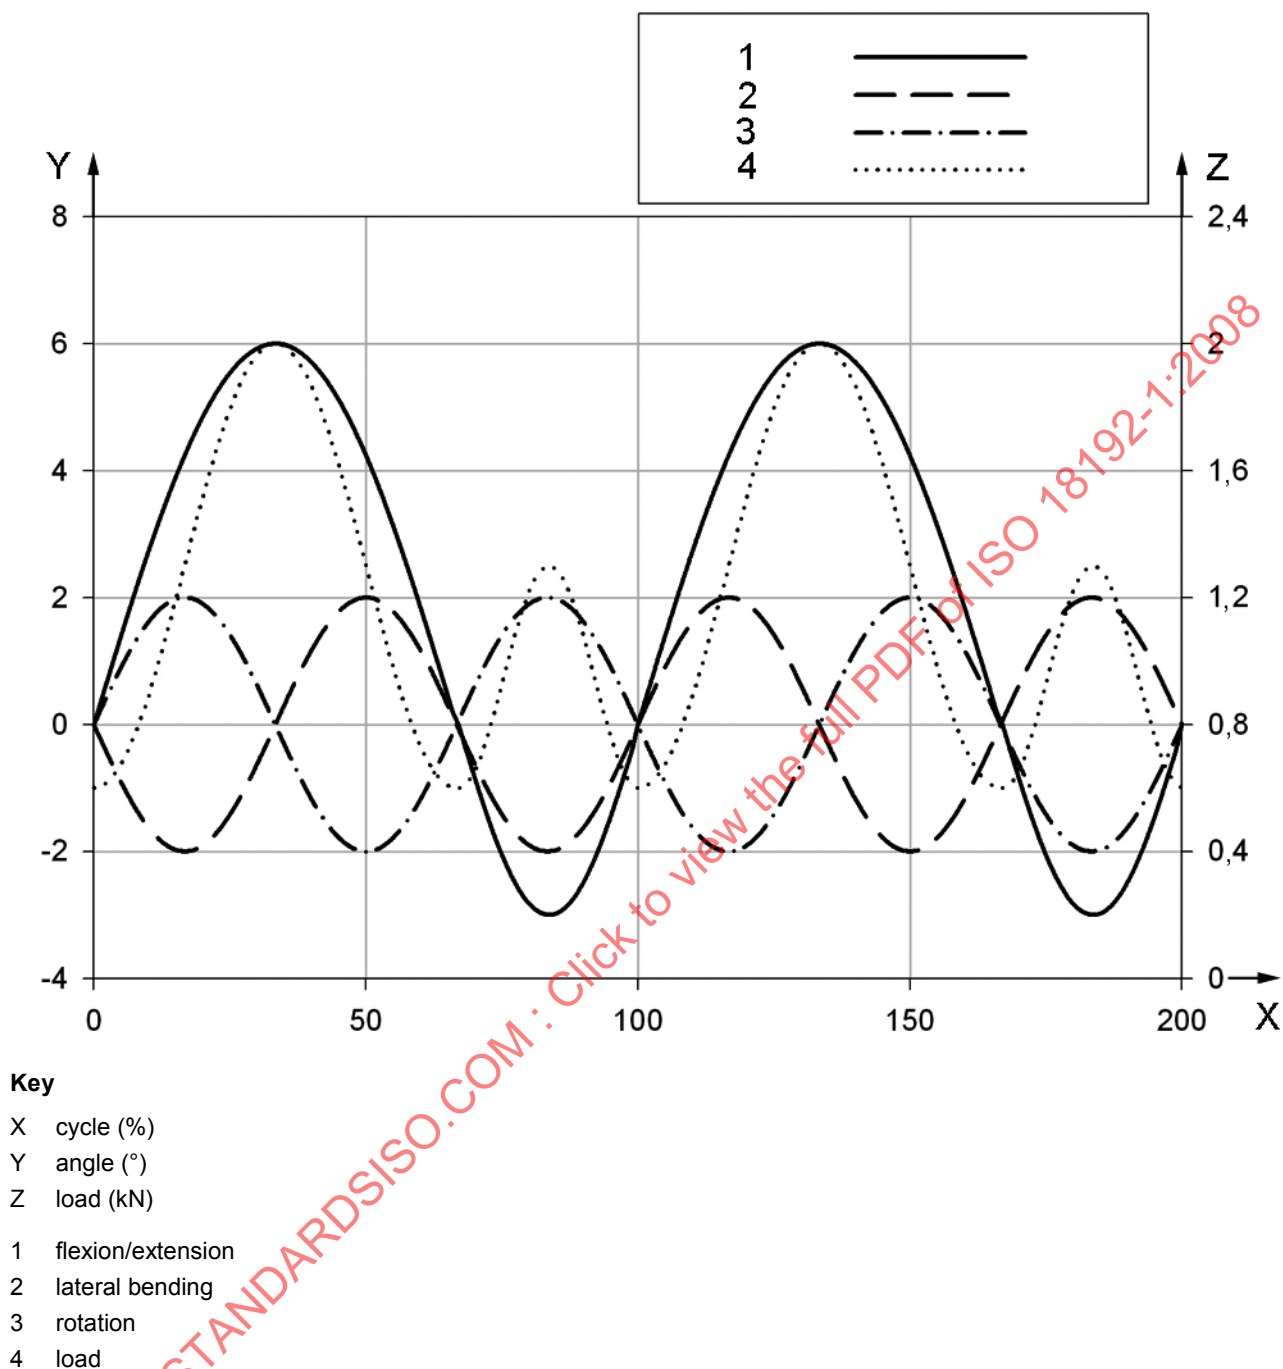

NOTE 100 % cycle corresponds to one cycle. The description of cycle given in 6.1 does not apply to Figure D.2.

**Figure D.2 — Phasing of the displacement and load curves (alternative) for lumbar prostheses**

## D.4 Alternative load and displacement data for cervical implants

Table D.1 — Alternative load and displacement data for cervical implants

| Loading cycle<br>(%) | Flexion/<br>extension<br>(°) | Lateral<br>bending<br>(°) | Rotation<br>(°) | Load<br>(N) | Loading cycle<br>(%) | Flexion/<br>extension<br>(°) | Lateral<br>bending<br>(°) | Rotation<br>(°) | Load<br>(N) |
|----------------------|------------------------------|---------------------------|-----------------|-------------|----------------------|------------------------------|---------------------------|-----------------|-------------|
| 0                    | 0,000                        | 0,000                     | 0,000           | 50,0        | 50                   | 7,071                        | 6,000                     | – 4,000         | 100,0       |
| 1                    | 0,471                        | – 0,565                   | 0,376           | 50,2        | 51                   | 6,730                        | 5,973                     | – 3,982         | 95,3        |
| 2                    | 0,941                        | – 1,124                   | 0,750           | 50,9        | 52                   | 6,374                        | 5,894                     | – 3,929         | 90,6        |
| 3                    | 1,409                        | – 1,674                   | 1,116           | 52,0        | 53                   | 6,004                        | 5,762                     | – 3,841         | 86,1        |
| 4                    | 1,874                        | – 2,209                   | 1,472           | 53,5        | 54                   | 5,621                        | 5,579                     | – 3,719         | 81,6        |
| 5                    | 2,334                        | – 2,724                   | 1,816           | 55,4        | 55                   | 5,225                        | 5,346                     | – 3,564         | 77,3        |
| 6                    | 2,790                        | – 3,215                   | 2,143           | 57,8        | 56                   | 4,818                        | 5,066                     | – 3,377         | 73,2        |
| 7                    | 3,239                        | – 3,677                   | 2,452           | 60,5        | 57                   | 4,399                        | 4,741                     | – 3,161         | 69,4        |
| 8                    | 3,681                        | – 4,107                   | 2,738           | 63,6        | 58                   | 3,971                        | 4,374                     | – 2,916         | 65,8        |
| 9                    | 4,115                        | – 4,501                   | 3,000           | 66,9        | 59                   | 3,535                        | 3,968                     | – 2,645         | 62,5        |
| 10                   | 4,540                        | – 4,854                   | 3,236           | 70,6        | 60                   | 3,090                        | 3,527                     | – 2,351         | 59,5        |
| 11                   | 4,955                        | – 5,164                   | 3,443           | 74,5        | 61                   | 2,639                        | 3,054                     | – 2,036         | 57,0        |
| 12                   | 5,358                        | – 5,429                   | 3,619           | 78,7        | 62                   | 2,181                        | 2,555                     | – 1,703         | 54,8        |
| 13                   | 5,750                        | – 5,645                   | 3,764           | 83,1        | 63                   | 1,719                        | 2,032                     | – 1,355         | 53,0        |
| 14                   | 6,129                        | – 5,811                   | 3,874           | 87,6        | 64                   | 1,253                        | 1,492                     | – 0,995         | 51,6        |
| 15                   | 6,494                        | – 5,926                   | 3,951           | 92,2        | 65                   | 0,785                        | 0,939                     | – 0,626         | 50,6        |
| 16                   | 6,845                        | – 5,988                   | 3,992           | 96,9        | 66                   | 0,314                        | 0,377                     | – 0,251         | 50,1        |
| 17                   | 7,181                        | – 5,997                   | 3,998           | 101,6       | 67                   | – 0,157                      | – 0,188                   | 0,126           | 50,0        |
| 18                   | 7,501                        | – 5,953                   | 3,968           | 106,3       | 68                   | – 0,627                      | – 0,752                   | 0,501           | 50,8        |
| 19                   | 7,804                        | – 5,856                   | 3,904           | 110,9       | 69                   | – 1,091                      | – 1,309                   | 0,873           | 52,4        |
| 20                   | 8,090                        | – 5,706                   | 3,804           | 115,5       | 70                   | – 1,545                      | – 1,854                   | 1,236           | 54,8        |
| 21                   | 8,358                        | – 5,507                   | 3,671           | 119,9       | 71                   | – 1,986                      | – 2,383                   | 1,589           | 57,9        |
| 22                   | 8,607                        | – 5,258                   | 3,505           | 124,1       | 72                   | – 2,409                      | – 2,891                   | 1,927           | 61,6        |
| 23                   | 8,838                        | – 4,962                   | 3,308           | 128,1       | 73                   | – 2,810                      | – 3,373                   | 2,248           | 65,8        |
| 24                   | 9,048                        | – 4,623                   | 3,082           | 131,9       | 74                   | – 3,187                      | – 3,825                   | 2,550           | 70,3        |
| 25                   | 9,239                        | – 4,243                   | 2,828           | 135,4       | 75                   | – 3,536                      | – 4,243                   | 2,828           | 75,0        |
| 26                   | 9,409                        | – 3,825                   | 2,550           | 138,5       | 76                   | – 3,853                      | – 4,623                   | 3,082           | 79,7        |
| 27                   | 9,558                        | – 3,373                   | 2,248           | 141,4       | 77                   | – 4,135                      | – 4,962                   | 3,308           | 84,2        |
| 28                   | 9,686                        | – 2,891                   | 1,927           | 143,8       | 78                   | – 4,382                      | – 5,258                   | 3,505           | 88,4        |
| 29                   | 9,792                        | – 2,383                   | 1,589           | 145,9       | 79                   | – 4,589                      | – 5,507                   | 3,671           | 92,1        |
| 30                   | 9,877                        | – 1,854                   | 1,236           | 147,6       | 80                   | – 4,755                      | – 5,706                   | 3,804           | 95,2        |
| 31                   | 9,940                        | – 1,309                   | 0,873           | 148,8       | 81                   | – 4,880                      | – 5,856                   | 3,904           | 97,6        |
| 32                   | 9,980                        | – 0,752                   | 0,501           | 149,6       | 82                   | – 4,961                      | – 5,953                   | 3,968           | 99,2        |

Table D.1 (continued)

| Loading cycle (%) | Flexion/extension (°) | Lateral bending (°) | Rotation (°) | Load (N) | Loading cycle (%) | Flexion/extension (°) | Lateral bending (°) | Rotation (°) | Load (N) |
|-------------------|-----------------------|---------------------|--------------|----------|-------------------|-----------------------|---------------------|--------------|----------|
| 33                | 9,999                 | – 0,188             | 0,126        | 150,0    | 83                | – 4,998               | – 5,997             | 3,998        | 100,0    |
| 34                | 9,995                 | 0,377               | – 0,251      | 149,9    | 84                | – 4,990               | – 5,988             | 3,992        | 99,8     |
| 35                | 9,969                 | 0,939               | – 0,626      | 149,4    | 85                | – 4,938               | – 5,926             | 3,951        | 98,8     |
| 36                | 9,921                 | 1,492               | – 0,995      | 148,4    | 86                | – 4,843               | – 5,811             | 3,874        | 96,9     |
| 37                | 9,851                 | 2,032               | – 1,355      | 147,0    | 87                | – 4,704               | – 5,645             | 3,764        | 94,3     |
| 38                | 9,759                 | 2,555               | – 1,703      | 145,2    | 88                | – 4,524               | – 5,429             | 3,619        | 90,9     |
| 39                | 9,646                 | 3,054               | – 2,036      | 143,0    | 89                | – 4,304               | – 5,164             | 3,443        | 87,0     |
| 40                | 9,511                 | 3,527               | – 2,351      | 140,5    | 90                | – 4,045               | – 4,854             | 3,236        | 82,7     |
| 41                | 9,354                 | 3,968               | – 2,645      | 137,5    | 91                | – 3,751               | – 4,501             | 3,000        | 78,1     |
| 42                | 9,178                 | 4,374               | – 2,916      | 134,2    | 92                | – 3,423               | – 4,107             | 2,738        | 73,4     |
| 43                | 8,980                 | 4,741               | – 3,161      | 130,6    | 93                | – 3,065               | – 3,677             | 2,452        | 68,8     |
| 44                | 8,763                 | 5,066               | – 3,377      | 126,8    | 94                | – 2,679               | – 3,215             | 2,143        | 64,4     |
| 45                | 8,526                 | 5,346               | – 3,564      | 122,7    | 95                | – 2,270               | – 2,724             | 1,816        | 60,3     |
| 46                | 8,271                 | 5,579               | – 3,719      | 118,4    | 96                | – 1,841               | – 2,209             | 1,472        | 56,8     |
| 47                | 7,997                 | 5,762               | – 3,841      | 113,9    | 97                | – 1,395               | – 1,674             | 1,116        | 53,9     |
| 48                | 7,705                 | 5,894               | – 3,929      | 109,4    | 98                | – 0,937               | – 1,124             | 0,750        | 51,8     |
| 49                | 7,396                 | 5,973               | – 3,982      | 104,7    | 99                | – 0,471               | – 0,565             | 0,376        | 0,000    |
| 100               | 0,000                 | 0,000               | 0,000        | 50,0     | 50,0              | 7,071                 | – 6,000             | 4,000        | 100,0    |
| 101               | 0,471                 | 0,565               | – 0,376      | 50,2     | 151               | 6,730                 | – 5,973             | 3,982        | 95,3     |
| 102               | 0,941                 | 1,124               | – 0,750      | 50,9     | 152               | 6,374                 | – 5,894             | 3,929        | 90,6     |
| 103               | 1,409                 | 1,674               | – 1,116      | 52,0     | 153               | 6,004                 | – 5,762             | 3,841        | 86,1     |
| 104               | 1,874                 | 2,209               | – 1,472      | 53,5     | 154               | 5,621                 | – 5,579             | 3,719        | 81,6     |
| 105               | 2,334                 | 2,724               | – 1,816      | 55,4     | 155               | 5,225                 | – 5,346             | 3,564        | 77,3     |
| 106               | 2,790                 | 3,215               | – 2,143      | 57,8     | 156               | 4,818                 | – 5,066             | 3,377        | 73,2     |
| 107               | 3,239                 | 3,677               | – 2,452      | 60,5     | 157               | 4,399                 | – 4,741             | 3,161        | 69,4     |
| 108               | 3,681                 | 4,107               | – 2,738      | 63,6     | 158               | 3,971                 | – 4,374             | 2,916        | 65,8     |
| 109               | 4,115                 | 4,501               | – 3,000      | 66,9     | 159               | 3,535                 | – 3,968             | 2,645        | 62,5     |
| 110               | 4,540                 | 4,854               | – 3,236      | 70,6     | 160               | 3,090                 | – 3,527             | 2,351        | 59,5     |
| 111               | 4,955                 | 5,164               | – 3,443      | 74,5     | 161               | 2,639                 | – 3,054             | 2,036        | 57,0     |
| 112               | 5,358                 | 5,429               | – 3,619      | 78,7     | 162               | 2,181                 | – 2,555             | 1,703        | 54,8     |
| 113               | 5,750                 | 5,645               | – 3,764      | 83,1     | 163               | 1,719                 | – 2,032             | 1,355        | 53,0     |
| 114               | 6,129                 | 5,811               | – 3,874      | 87,6     | 164               | 1,253                 | – 1,492             | 0,995        | 51,6     |
| 115               | 6,494                 | 5,926               | – 3,951      | 92,2     | 165               | 0,785                 | – 0,939             | 0,626        | 50,6     |
| 116               | 6,845                 | 5,988               | – 3,992      | 96,9     | 166               | 0,314                 | – 0,377             | 0,251        | 50,1     |
| 117               | 7,181                 | 5,997               | – 3,998      | 101,6    | 167               | – 0,157               | 0,188               | – 0,126      | 50,0     |

Table D.1 (continued)

| Loading cycle (%)                            | Flexion/extension (°) | Lateral bending (°) | Rotation (°) | Load (N) | Loading cycle (%) | Flexion/extension (°) | Lateral bending (°) | Rotation (°) | Load (N) |
|----------------------------------------------|-----------------------|---------------------|--------------|----------|-------------------|-----------------------|---------------------|--------------|----------|
| 118                                          | 7,501                 | 5,953               | – 3,968      | 106,3    | 168               | – 0,627               | 0,752               | – 0,501      | 50,8     |
| 119                                          | 7,804                 | 5,856               | – 3,904      | 110,9    | 169               | – 1,091               | 1,309               | – 0,873      | 52,4     |
| 120                                          | 8,090                 | 5,706               | – 3,804      | 115,5    | 170               | – 1,545               | 1,854               | – 1,236      | 54,8     |
| 121                                          | 8,358                 | 5,507               | – 3,671      | 119,9    | 171               | – 1,986               | 2,383               | – 1,589      | 57,9     |
| 122                                          | 8,607                 | 5,258               | – 3,505      | 124,1    | 172               | – 2,409               | 2,891               | – 1,927      | 61,6     |
| 123                                          | 8,838                 | 4,962               | – 3,308      | 128,1    | 173               | – 2,810               | 3,373               | – 2,248      | 65,8     |
| 124                                          | 9,048                 | 4,623               | – 3,082      | 131,9    | 174               | – 3,187               | 3,825               | – 2,550      | 70,3     |
| 125                                          | 9,239                 | 4,243               | – 2,828      | 135,4    | 175               | – 3,536               | 4,243               | – 2,828      | 75,0     |
| 126                                          | 9,409                 | 3,825               | – 2,550      | 138,5    | 176               | – 3,853               | 4,623               | – 3,082      | 79,7     |
| 127                                          | 9,558                 | 3,373               | – 2,248      | 141,4    | 177               | – 4,135               | 4,962               | – 3,308      | 84,2     |
| 128                                          | 9,686                 | 2,891               | – 1,927      | 143,8    | 178               | – 4,382               | 5,258               | – 3,505      | 88,4     |
| 129                                          | 9,792                 | 2,383               | – 1,589      | 145,9    | 179               | – 4,589               | 5,507               | – 3,671      | 92,1     |
| 130                                          | 9,877                 | 1,854               | – 1,236      | 147,6    | 180               | – 4,755               | 5,706               | – 3,804      | 95,2     |
| 131                                          | 9,940                 | 1,309               | – 0,873      | 148,8    | 181               | – 4,880               | 5,856               | – 3,904      | 97,6     |
| 132                                          | 9,980                 | 0,752               | – 0,501      | 149,6    | 182               | – 4,961               | 5,953               | – 3,968      | 99,2     |
| 133                                          | 9,999                 | 0,188               | – 0,126      | 150,0    | 183               | – 4,998               | 5,997               | – 3,998      | 100,0    |
| 134                                          | 9,995                 | – 0,377             | 0,251        | 149,9    | 184               | – 4,990               | 5,988               | – 3,992      | 99,8     |
| 135                                          | 9,969                 | – 0,939             | 0,626        | 149,4    | 185               | – 4,938               | 5,926               | – 3,951      | 98,8     |
| 136                                          | 9,921                 | – 1,492             | 0,995        | 148,4    | 186               | – 4,843               | 5,811               | – 3,874      | 96,9     |
| 137                                          | 9,851                 | – 2,032             | 1,355        | 147,0    | 187               | – 4,704               | 5,645               | – 3,764      | 94,3     |
| 138                                          | 9,759                 | – 2,555             | 1,703        | 145,2    | 188               | – 4,524               | 5,429               | – 3,619      | 90,9     |
| 139                                          | 9,646                 | – 3,054             | 2,036        | 143,0    | 189               | – 4,304               | 5,164               | – 3,443      | 87,0     |
| 140                                          | 9,511                 | – 3,527             | 2,351        | 140,5    | 190               | – 4,045               | 4,854               | – 3,236      | 82,7     |
| 141                                          | 9,354                 | – 3,968             | 2,645        | 137,5    | 191               | – 3,751               | 4,501               | – 3,000      | 78,1     |
| 142                                          | 9,178                 | – 4,374             | 2,916        | 134,2    | 192               | – 3,423               | 4,107               | – 2,738      | 73,4     |
| 143                                          | 8,980                 | – 4,741             | 3,161        | 130,6    | 193               | – 3,065               | 3,677               | – 2,452      | 68,8     |
| 144                                          | 8,763                 | – 5,066             | 3,377        | 126,8    | 194               | – 2,679               | 3,215               | – 2,143      | 64,4     |
| 145                                          | 8,526                 | – 5,346             | 3,564        | 122,7    | 195               | – 2,270               | 2,724               | – 1,816      | 60,3     |
| 146                                          | 8,271                 | – 5,579             | 3,719        | 118,4    | 196               | – 1,841               | 2,209               | – 1,472      | 56,8     |
| 147                                          | 7,997                 | – 5,762             | 3,841        | 113,9    | 197               | – 1,395               | 1,674               | – 1,116      | 53,9     |
| 148                                          | 7,705                 | – 5,894             | 3,929        | 109,4    | 198               | – 0,937               | 1,124               | – 0,750      | 51,8     |
| 149                                          | 7,396                 | – 5,973             | 3,982        | 104,7    | 199               | – 0,471               | 0,565               | – 0,376      | 50,4     |
| NOTE 100 % loading cycle corresponds to 1 s. |                       |                     |              |          |                   |                       |                     |              |          |

## D.5 Alternative load and displacement data for lumbar implants

Table D.2 — Alternative load and displacement data for lumbar implants

| Loading cycle<br>(%) | Flexion/<br>extension<br>(°) | Lateral<br>bending<br>(°) | Rotation<br>(°) | Load<br>(kN) | Loading cycle<br>(%) | Flexion/<br>extension<br>(°) | Lateral<br>bending<br>(°) | Rotation<br>(°) | Load<br>(kN) |
|----------------------|------------------------------|---------------------------|-----------------|--------------|----------------------|------------------------------|---------------------------|-----------------|--------------|
| 0                    | 0,000                        | 0,000                     | 0,000           | 0,600        | 50                   | 4,243                        | 2,000                     | – 2,000         | 1,300        |
| 1                    | 0,283                        | – 0,188                   | 0,188           | 0,603        | 51                   | 4,038                        | 1,991                     | – 1,991         | 1,234        |
| 2                    | 0,565                        | – 0,375                   | 0,375           | 0,612        | 52                   | 3,825                        | 1,965                     | – 1,965         | 1,169        |
| 3                    | 0,845                        | – 0,558                   | 0,558           | 0,628        | 53                   | 3,603                        | 1,921                     | – 1,921         | 1,105        |
| 4                    | 1,124                        | – 0,736                   | 0,736           | 0,649        | 54                   | 3,373                        | 1,860                     | – 1,860         | 1,042        |
| 5                    | 1,401                        | – 0,908                   | 0,908           | 0,676        | 55                   | 3,135                        | 1,782                     | – 1,782         | 0,982        |
| 6                    | 1,674                        | – 1,072                   | 1,072           | 0,709        | 56                   | 2,891                        | 1,689                     | – 1,689         | 0,925        |
| 7                    | 1,944                        | – 1,226                   | 1,226           | 0,747        | 57                   | 2,640                        | 1,580                     | – 1,580         | 0,871        |
| 8                    | 2,209                        | – 1,369                   | 1,369           | 0,790        | 58                   | 2,383                        | 1,458                     | – 1,458         | 0,821        |
| 9                    | 2,469                        | – 1,500                   | 1,500           | 0,837        | 59                   | 2,121                        | 1,323                     | – 1,323         | 0,775        |
| 10                   | 2,724                        | – 1,618                   | 1,618           | 0,889        | 60                   | 1,854                        | 1,176                     | – 1,176         | 0,734        |
| 11                   | 2,973                        | – 1,721                   | 1,721           | 0,944        | 61                   | 1,583                        | 1,018                     | – 1,018         | 0,697        |
| 12                   | 3,215                        | – 1,810                   | 1,810           | 1,002        | 62                   | 1,309                        | 0,852                     | – 0,852         | 0,667        |
| 13                   | 3,450                        | – 1,882                   | 1,882           | 1,063        | 63                   | 1,032                        | 0,677                     | – 0,677         | 0,641        |
| 14                   | 3,677                        | – 1,937                   | 1,937           | 1,126        | 64                   | 0,752                        | 0,497                     | – 0,497         | 0,622        |
| 15                   | 3,897                        | – 1,975                   | 1,975           | 1,190        | 65                   | 0,471                        | 0,313                     | – 0,313         | 0,609        |
| 16                   | 4,107                        | – 1,996                   | 1,996           | 1,256        | 66                   | 0,188                        | 0,126                     | – 0,126         | 0,601        |
| 17                   | 4,309                        | – 1,999                   | 1,999           | 1,322        | 67                   | 0,000                        | – 0,063                   | 0,063           | 0,600        |
| 18                   | 4,501                        | – 1,984                   | 1,984           | 1,388        | 68                   | – 0,282                      | – 0,251                   | 0,251           | 0,606        |
| 19                   | 4,683                        | – 1,952                   | 1,952           | 1,453        | 69                   | – 0,562                      | – 0,436                   | 0,436           | 0,625        |
| 20                   | 4,854                        | – 1,902                   | 1,902           | 1,516        | 70                   | – 0,837                      | – 0,618                   | 0,618           | 0,654        |
| 21                   | 5,015                        | – 1,836                   | 1,836           | 1,578        | 71                   | – 1,104                      | – 0,794                   | 0,794           | 0,695        |
| 22                   | 5,164                        | – 1,753                   | 1,753           | 1,637        | 72                   | – 1,362                      | – 0,964                   | 0,964           | 0,744        |
| 23                   | 5,303                        | – 1,654                   | 1,654           | 1,693        | 73                   | – 1,607                      | – 1,124                   | 1,124           | 0,801        |
| 24                   | 5,429                        | – 1,541                   | 1,541           | 1,746        | 74                   | – 1,839                      | – 1,275                   | 1,275           | 0,863        |
| 25                   | 5,543                        | – 1,414                   | 1,414           | 1,795        | 75                   | – 2,054                      | – 1,414                   | 1,414           | 0,928        |
| 26                   | 5,645                        | – 1,275                   | 1,275           | 1,839        | 76                   | – 2,250                      | – 1,541                   | 1,541           | 0,994        |
| 27                   | 5,735                        | – 1,124                   | 1,124           | 1,879        | 77                   | – 2,427                      | – 1,654                   | 1,654           | 1,058        |
| 28                   | 5,811                        | – 0,964                   | 0,964           | 1,913        | 78                   | – 2,582                      | – 1,753                   | 1,753           | 1,119        |
| 29                   | 5,875                        | – 0,794                   | 0,794           | 1,942        | 79                   | – 2,714                      | – 1,836                   | 1,836           | 1,173        |
| 30                   | 5,926                        | – 0,618                   | 0,618           | 1,966        | 80                   | – 2,823                      | – 1,902                   | 1,902           | 1,220        |
| 31                   | 5,964                        | – 0,436                   | 0,436           | 1,983        | 81                   | – 2,906                      | – 1,952                   | 1,952           | 1,257        |
| 32                   | 5,988                        | – 0,251                   | 0,251           | 1,994        | 82                   | – 2,963                      | – 1,984                   | 1,984           | 1,283        |