



**International
Standard**

ISO 20336

**Coal and coke — Determination
of total sulfur by Coulomb
titration method**

*Charbon et coke — Détermination de la teneur totale en soufre
par la méthode de titrage de Coulomb*

**Second edition
2025-02**

STANDARDSISO.COM : Click to view the full PDF of ISO 20336:2025



COPYRIGHT PROTECTED DOCUMENT

© ISO 2025

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: +41 22 749 01 11
Email: copyright@iso.org
Website: www.iso.org

Published in Switzerland

Contents

Page

Foreword	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Principle	1
5 Reagent and materials	1
6 Apparatus	2
7 Preparation of test sample	4
8 Procedure	5
8.1 Preparation of test	5
8.2 Calibration	5
8.3 Calibration procedure	5
8.4 Procedure	6
8.5 Calibration check	6
9 Expression of result	6
10 Precision	7
10.1 Repeatability limit	7
10.2 Reproducibility limit	7
11 Test report	7

STANDARDSISO.COM : Click to view the full PDF of ISO 20336:2025

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO document should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

ISO draws attention to the possibility that the implementation of this document may involve the use of (a) patent(s). ISO takes no position concerning the evidence, validity or applicability of any claimed patent rights in respect thereof. As of the date of publication of this document, ISO had not received notice of (a) patent(s) which may be required to implement this document. However, implementers are cautioned that this may not represent the latest information, which may be obtained from the patent database available at www.iso.org/patents. ISO shall not be held responsible for identifying any or all such patent rights.

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 27, *Coal and coke*, Subcommittee SC 5, *Methods of analysis*.

This second edition cancels and replaces the first edition (ISO 20336:2017), which has been technically revised.

The main changes are as follows:

- replaced “solid mineral fuels” with “coal and coke” and “content” with “mass fraction”;
- added [Figure 2](#) of a purified air stream supply system;
- added a note to [8.1.4](#).

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html

Introduction

The objective of this document is to provide an alternative method for determining the total sulfur mass fraction in coal and coke with high-temperature combustion by Coulomb titration using automated instruments.

STANDARDSISO.COM : Click to view the full PDF of ISO 20336:2025

STANDARDSISO.COM : Click to view the full PDF of ISO 20336:2025

Coal and coke — Determination of total sulfur by Coulomb titration method

1 Scope

This document specifies an alternative method of determining the total sulfur mass fraction of coal and coke by high-temperature combustion by Coulomb titration.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 687, *Coke — Determination of moisture in the general analysis test sample*

ISO 5068-2, *Brown coals and lignites — Determination of moisture content — Part 2: Indirect gravimetric method for moisture in the analysis sample*

ISO 11722, *Solid mineral fuels — Hard coal — Determination of moisture in the general analysis test sample by drying in nitrogen*

3 Terms and definitions

No terms and definitions are listed in this document.

ISO and IEC maintain terminology databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <https://www.electropedia.org/>

4 Principle

In the presence of the catalyst, a sample of known mass is combusted at 1 150 °C in a stream of purified air. The sulfur oxides are formed and dissolved in the electrolytic solution. The sulfur dioxides are titrated by the iodine and bromine liberated from the electrolysis of the potassium iodide and potassium bromide solution. The quantity of the electricity consumed by electrolysis is integrated and used to calculate the mass fraction of sulfur dioxides. The instrument is calibrated with certified reference materials. The percentage of total sulfur in the sample is calculated according to the sulfur dioxides mass fraction and the prior calibration.

5 Reagent and materials

During the analysis, unless otherwise stated, use only reagents of recognized analytical grade and only distilled water or water of equivalent purity.

5.1 Potassium iodide.

5.2 Potassium bromide.

5.3 Glacial acetic acid.

5.4 Self-indicating silica gel, industrial grade.

5.5 Sodium hydroxide, chemical grade.

5.6 Electrolytic solution, composed of 5 g of potassium iodide (5.1) and 5 g of potassium bromide (5.2) dissolved in (250 to 300) ml of water, then add 10 ml of glacial acetic acid.

5.7 Glass wool.

5.8 Aluminosilicate wool.

5.9 Catalyst, tungsten trioxide.

5.10 Certified reference materials (CRMs), coal or coke.

6 Apparatus

6.1 Instrument, for determining sulfur by Coulomb titration, commercially available, consisting of the following (see Figure 1).

6.2 Tube resistance furnace and combustion tube, capable of maintaining a temperature of $(1\ 150 \pm 10)$ °C in the combustion zone which is at least 70 mm long, with the Pt-Rh-Pt thermocouple and the temperature controller. The combustion tube is made of silicon or corundum, capable of withstanding temperatures greater than 1 300 °C.

6.3 Electrolytic cell and magnetic stirrer.

The electrolytic cell consists of a cylindrical glass cup of over 400 ml capacity, with (120 to 180) mm high, in which there are a pair of Pt electrolytic electrodes each of 150 mm² area and a pair of Pt indicating electrodes each of 15 mm² area. The response time of indicating electrodes should be less than 1 s. The magnetic stirrer with speed of 500 r/min and regulator is also provided.

6.4 Coulomb integrator.

The integration linearity error is less than 0,1 % at (0 to 350) mA of electrolyzing current, with a (4 to 6 digit) digital display or printer to give the mass fraction of the sulfur in the sample.

6.5 Program controller.

The sample can be pushed into and withdrawn from the combustion tube according to the specified program.

6.6 Purified air stream supply system, consisting of magnetic pumps and purifying tubes and a flowmeter.


Supply an air stream at the rate of 1 500 ml/min and aspirating it at 1 000 ml/min (indicating by a flowmeter), which is purified and dried by the sodium hydroxide and self-indicating silica gel packed in the purifying tubes respectively (see Figure 2).

NOTE The sodium hydroxide is not necessary for the laboratories in which the air is not polluted by acid gas.

6.7 Combustion boat, made of unglazed porcelain or quartz, about 60 mm long at the part of packing the sample, capable of withstanding over 1 200 °C.

6.8 Quartz tray, capable of withstanding over 1 200 °C and supporting the combustion boat moving in and out the combustion tube.


6.9 Analytical balance, having a resolution of 0,1 mg.

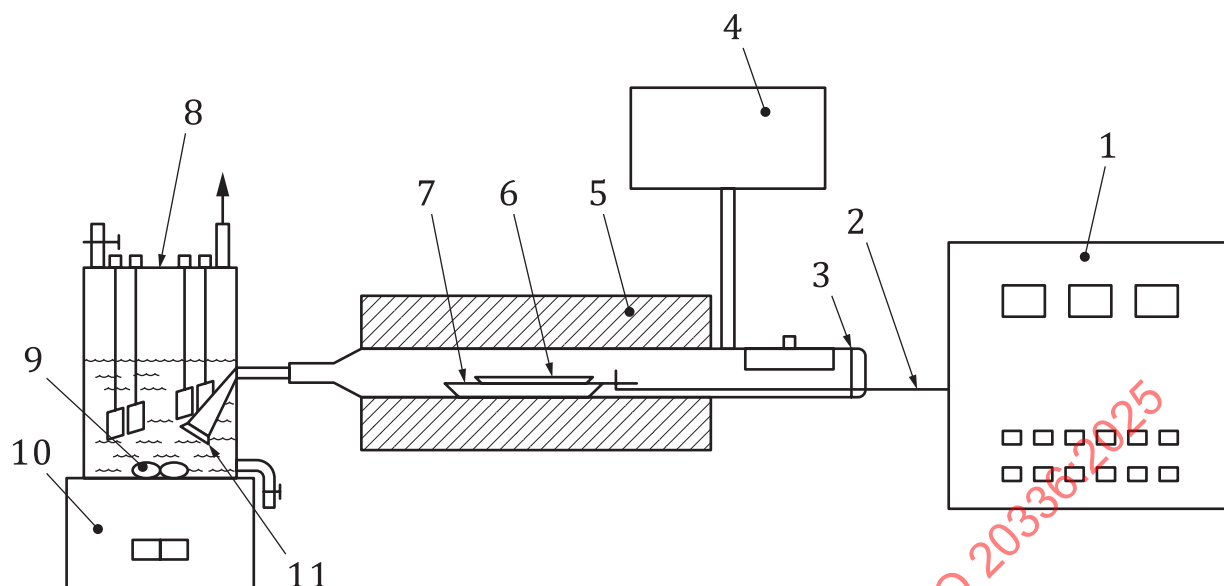

Key

- 1 program controller
- 2 pulling stem
- 3 combustion tube
- 4 purified device for air stream
- 5 resistance furnace
- 6 sample boat
- 7 quartz tray
- 8 electrolytic cell
- 9 stirrer stem
- 10 magnetic stirrer
- 11 gas filter

Figure 1 — Equipment for determining sulfur by Coulomb titration

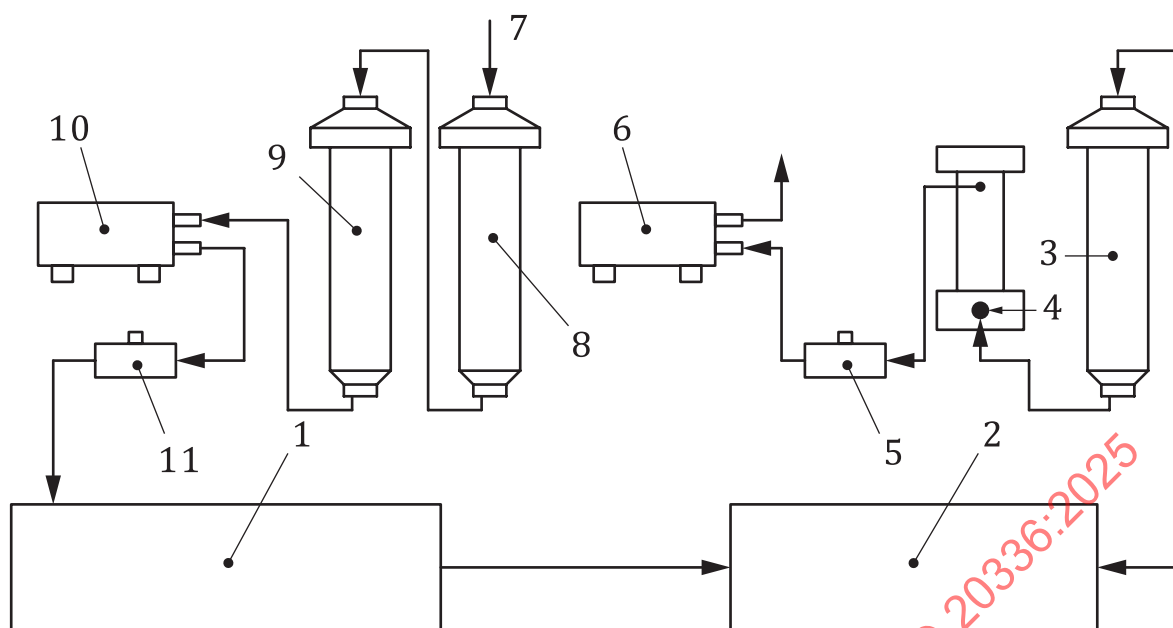**Key**

- 1 tube resistance furnace and combustion tube
- 2 electrolytic cell
- 3 silica gel
- 4 flow meter, 1 000 mL/min
- 5 regulator
- 6 pump
- 7 air
- 8 silica gel
- 9 NaOH
- 10 pump
- 11 regulator

Figure 2 — Purified air stream supply system**7 Preparation of test sample**

The coal or coke used for the determination of total sulfur is the general analysis test sample ground to pass a sieve of 212 μm aperture, and for the coal or coke with sulfur higher than 5 % of the sulfur, the general analysis test sample is ground to pass a sieve of 100 μm aperture.

Expose the sample in a thin layer for the minimum time required for the moisture mass fraction to reach to approximate equilibrium with the laboratory atmosphere. Before commencing the determination, thoroughly mix the air-dried sample.

If the results are to be calculated other than on an "air-dried basis", then, after determining the test portion mass (see 8.4.4), the moisture mass fraction shall be determined using a further portion of the test sample by the method specified in ISO 687, ISO 5068-2 or ISO 11722.

8 Procedure

8.1 Preparation of test

8.1.1 Raise the temperature of the furnace to $1\,150\text{ }^{\circ}\text{C}$. Measure the position and length of high temperature zone of $(1\,150 \pm 10)\text{ }^{\circ}\text{C}$ and the position of preliminary decomposition zone of $500\text{ }^{\circ}\text{C}$ in combustion tube using a calibrated pyrometer with Pt-Rh-Pt thermocouple.

8.1.2 Adjust the program controller to ensure the combustion boat moves into the position of the preliminary decomposition zone of $500\text{ }^{\circ}\text{C}$ and then to the combustion zone of $1\,150\text{ }^{\circ}\text{C}$ automatically.

8.1.3 Fill the clean and dry glass wool (5.7) in the exit end of the combustion tube. Fill the (3 to 5) mm thickness of aluminosilicate wool (5.8) in the area of (80 to 100) mm from the exit end of the combustion tube.

8.1.4 Assemble tube resistance furnace (6.2) with a combustion tube (6.2), electrolytic cell (6.3), magnetic stirrer (6.3), coulomb integrator (6.4), the program controller (6.5), and the purified air stream supply system (6.6). The combustion tube, stopcock and electrolytic cell should be connected in glass to glass closely and sealed with silicone rubber sleeves.

NOTE The assembly and integration processes are usually completed by the manufacturer.

8.1.5 Switch on the pump and adjust aspirating rate of air to $1\,000\text{ ml/min}$, then close the stopcock between the electrolytic cell and the combustion tube. If the aspirating rate of air drops down under 300 ml/min , it indicates that all of parts and joints of the instrument are gas tight. Otherwise, check for the leaks in the system.

8.2 Calibration

Calibrate the instrument according to one of following two methods using the CRMs (5.10) of coal or coke:

a) Multi-point calibration method.

Calibrate the instrument with at least three CRMs (5.10) of coal or coke that cover the range of sulfur mass fractions that represent the samples.

b) Single-point calibration method.

Calibration is made with a CRM of coal or coke, in which the sulfur mass fraction is similar to that in the sample.

8.3 Calibration procedure

8.3.1 Determine the moisture of the CRMs of coal or coke (see Clause 7) used as part of the calibration in accordance with drying instructions on the CRM certificate, and by which the air-dried basis of the total sulfur mass fraction of the CRMs are calculated.

8.3.2 Check the instrument to ensure that it is in the normal condition before calibration. Determine the total sulfur mass fraction of the CRMs of coal or coke in accordance with the procedures specified in 8.4. Run a minimum of three times (in triplicate) for every sample. Take the mean value of the replicates as the determined value for sulfur. The replicate results shall agree within the repeatability limit specified in 10.1, if not, check the instrument and repeat the calibration tests.

8.3.3 The calibration factor is calculated from the determined values and the certified values of the CRMs which are calculated to the air-dried basis.

For some instruments, the calibration factors need to be calculated and then put into the instrument manually.