
**Implants for surgery — In vitro
evaluation for apatite-forming ability
of implant materials**

*Implants chirurgicaux — Évaluation in vitro de la capacité de
formation d'apatite des matériaux d'implants*

STANDARDSISO.COM : Click to view the full PDF of ISO 23317:2014



STANDARDSISO.COM : Click to view the full PDF of ISO 23317:2014



COPYRIGHT PROTECTED DOCUMENT

© ISO 2014

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

Page

Foreword	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Apparatus	2
5 Test specimen	2
5.1 Specimen configuration and size	2
5.2 Specimen preparation	2
6 Simulated body fluid	3
6.1 General.....	3
6.2 Reagents for SBF.....	3
6.3 Preparation of SBF	4
6.4 Confirmation of ion concentration of SBF	6
6.5 Preservation of SBF	6
7 Procedure	6
8 Test report	8
Annex A (informative) Apparatus for preparing SBF	9
Annex B (informative) Preparation of standard glasses for evaluating apatite-forming ability	10
Bibliography	12

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT) see the following URL: Foreword - Supplementary information

The committee responsible for this document is ISO/TC 150, *Implants for surgery*, Subcommittee SC 1, *Materials*.

This third edition cancels and replaces the second edition (ISO 23317:2012), which has been editorially revised.

Introduction

It has been revealed that materials of various kinds bond to living bone through a layer of apatite. It has been shown that this apatite layer can be reproduced on their surfaces in an acellular and protein-free simulated body fluid (SBF) with ion concentrations nearly equal to those of human blood plasma, and that apatite thus formed is similar to the bone mineral in its composition and structure.

This evaluation of apatite-forming ability on implant material in SBF is useful for evaluating its *in vivo* bone-bonding ability preliminary to animal experiments. When a bioactive material is implanted in a living body, a thin layer rich in Ca and P forms on its surface. The material then connects to the living tissue through this apatite layer without a distinct boundary. It has been shown that this apatite layer can be reproduced on the surfaces of materials in SBF as well, and that apatite thus formed is similar to bone mineral in its composition and structure. As bioactivity increases, apatite forms on the material surface in a shorter time in proportion to this increase. The formation of apatite layers can be detected by thin film X-ray diffraction spectrometry and/or scanning electron microscopy.

The apatite formed in the SBF is, however, similar to bone apatite in the following points.

- Ca-deficient type apatite.
- Lower Ca/P atomic ratio than stoichiometric apatite.
- Containing some impurities such as Mg^{2+} , Na^+ , Cl^- , HCO_3^- .
- Low crystallinity.

NOTE 1 The material which forms apatite on its surface *in vivo* can bond to living bone, since this apatite is biologically active. Their *in vivo* apatite deposition can be reproduced on their surfaces even *in vitro* in SBF. For example, *in vivo* calcification on surfaces of Bioglass®¹⁾, CaO-SiO₂ glasses, Na₂O-CaO-SiO₂ glasses, Cerabone®²⁾ A-W, Ceravital®³⁾ -type glass-ceramic, sintered hydroxyapatite and alkali-heat-treated titanium metal, are correlated with *in vitro* calcification in SBF. However, this does not exclude the possibility that materials, which do not form apatite on their surfaces *in vivo*, bond to living bone. For example, it is reported that such resorbable materials as beta-tricalcium phosphate (Ca₃(PO₄)₂) and calcium carbonate bond to living bone without forming an apatite layer on their surfaces.

NOTE 2 It has been reported that glasses with different compositions in the system Na₂O-CaO-SiO₂ show a correlation between bone-forming ability of materials implanted into a bone defect of a rabbit and apatite-forming ability on its surface in SBF.

1) Trade names of products are an example of a suitable product available commercially. This information is given for the convenience of users of this document and does not constitute an endorsement by ISO of this product.

2) Trade names of products are an example of a suitable product available commercially. This information is given for the convenience of users of this document and does not constitute an endorsement by ISO of this product.

3) Trade names of products are an example of a suitable product available commercially. This information is given for the convenience of users of this document and does not constitute an endorsement by ISO of this product.

STANDARDSISO.COM : Click to view the full PDF of ISO 23317:2014

Implants for surgery — In vitro evaluation for apatite-forming ability of implant materials

1 Scope

This International Standard specifies a method for detecting apatite formed on a surface of a material in simulated body fluid (SBF). It is applicable to implant surfaces intended to come into direct bone contact.

2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 3696:1987, *Water for analytical laboratory use — Specification and test methods*

ISO 14630, *Non-active surgical implants — General requirements*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 14630 and the following apply.

3.1

apatite

group of calcium-phosphates including bone mineral and the main inorganic constituent of bones and teeth similar to hydroxyapatite, which has the composition $\text{Ca}_{10}(\text{PO}_4)_6(\text{OH})_2$

Note 1 to entry: Bone mineral also contains ions such as CO_3^{2-} , F^- , Na^+ and Mg^{2+} .

3.2

apatite-forming ability

capability to develop apatite on the surface

3.3

bioactivity

property that elicits a specific biological response at the interface of the material, which results in the formation of a bond between tissue and material

3.4

induction period

time to detect apatite formation on a surface of a specimen after soaking the specimen in simulated body fluid

3.5

simulated body fluid

SBF

inorganic solution having a similar composition to human blood plasma without organic components

3.6

standard glass for evaluating apatite-forming ability

class of standard glasses with certain chemical compositions as shown in [Annex B](#) showing given apatite-forming abilities in SBF and when implanted in an animal body

3.7 thin film X-ray diffraction spectrometry TF-XRD

method for detecting minerals in a thin layer at the surface of a material from a diffraction pattern obtained by X-ray with small glancing angle against the surface of the sample

4 Apparatus

4.1 Electric balance, capable of measuring a mass with an accuracy of ± 1 mg.

4.2 Water bath equipped with magnetic stirrer, to maintain temperature of the solution within the range of $(36,5 \pm 2)$ °C and an accuracy of $\pm 0,2$ °C.

4.3 pH meter, capable of measuring the pH of a solution with an accuracy of $\pm 0,01$.

4.4 Thermometer, capable of measuring the temperature of a solution with an accuracy of $\pm 0,1$ °C.

4.5 Thin film X-ray diffraction spectrometer (TF-XRD), capable of detecting apatite formed in a thin layer at the surface of a material.

4.6 Scanning electron microscope (SEM), capable of observing apatite grains and/or layers formed on a plain surface of a material with a magnification up to $\times 10\,000$.

5 Test specimen

5.1 Specimen configuration and size

This International Standard allows specimens of any configuration and size derived from implant parts and devices to be used. However, a disc or rectangular plate specimen is highly recommended, because bioactivity of a material is evaluated by confirmation of apatite formed on the surface of the material using TF-XRD and/or SEM. Recommended specimen dimensions are shown in [Figure 1](#).

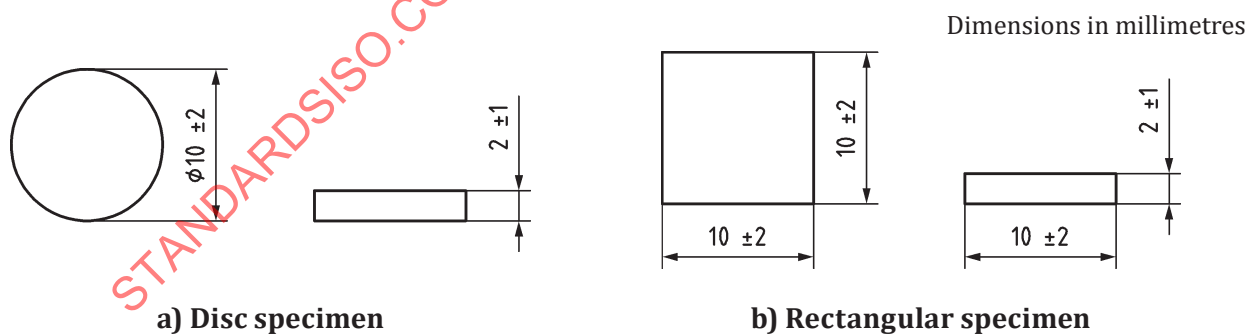


Figure 1 — Recommended specimen dimensions

5.2 Specimen preparation

5.2.1 General

This International Standard allows several options for specimen preparation. The specimens should be machined, if necessary, to alter the configurations of original implants.

5.2.2 Basic machining procedure

In the case of a rectangular thin plate specimen as shown in [Figure 1 b](#), the following procedure shall be used. Specimens shall be ground using a diamond wheel of grit size between 120 and 400. Conditions such as depth of cut per pass, wheel speed and others depend on the ground material. Water soluble materials, such as bioactive standard glasses, shall be machined under non-aqueous conditions.

Where a customary machining procedure has been developed that is completely satisfactory for apatite-forming ability testing, this customary procedure can be used.

6 Simulated body fluid

6.1 General

Simulated body fluid (SBF) as defined in [Table 1](#) shall be used.

Table 1 — Ion concentrations of SBF and human blood plasma

Ion	Concentration (10^{-3} mol) in	
	SBF (pH 7,40)	Blood plasma (pH 7,2 to 7,4)
Na ⁺	142,0	142,0
K ⁺	5,0	5,0
Mg ²⁺	1,5	1,5
Ca ²⁺	2,5	2,5
Cl ⁻	147,8	103,0
HCO ₃ ⁻	4,2	27,0
HPO ₄ ²⁻	1,0	1,0
SO ₄ ²⁻	0,5	0,5

NOTE 1 For SBF as defined in [Table 1](#), a correlation was observed between *in vivo* bone ingrowth and *in vitro* apatite-forming ability.

NOTE 2 Other kinds of SBFs have been proposed in the literature, some of which have shown a correlation between *in vivo* bone ingrowth and *in vitro* apatite-forming ability.

6.2 Reagents for SBF

For the preparation of SBF only reagents of the following recognized analytical grade chemicals and only water in accordance with ISO 3696:1987, grade 2, shall be used.

6.2.1 Sodium chloride (NaCl)

6.2.2 Sodium hydrogen carbonate (NaHCO₃)

6.2.3 Potassium chloride (KCl)

6.2.4 Di-potassium hydrogen phosphate trihydrate (K₂HPO₄ • 3H₂O)

6.2.5 Magnesium chloride hexahydrate (MgCl₂ • 6H₂O)

6.2.6 Hydrochloric acid solution, $c(\text{HCl}) = 1 \text{ mol/l}$.

6.2.7 Calcium chloride (CaCl_2) or calcium chloride dihydrate ($\text{CaCl}_2 \cdot 2\text{H}_2\text{O}$)

6.2.8 Sodium sulfate (Na_2SO_4)

6.2.9 Tris-hydroxymethyl aminomethane (TRIS): $((\text{HOCH}_2)_3\text{CNH}_2)$

6.3 Preparation of SBF

6.3.1 General

Since SBF is supersaturated with respect to apatite, an inappropriate preparation method can lead to the homogeneous precipitation of apatite in the solution.

During its preparation the solution shall remain colourless, transparent and without deposit on the surface of the bottle. If any precipitation occurs, stop preparing SBF, abandon the solution and restart by washing the apparatus.

In [Table 2](#), the reagents for the preparation of 1 l of SBF are given in the required order of dissolution.

Table 2 — Ion concentrations of SBF and human blood plasma

Order	Reagent	Amount ^a	Container	Purity ^b	Formula weight
1	6.2.1	8,035 g	weighing paper	99,5 %	58,443 0
2	6.2.2	0,355 g	weighing paper	99,5 %	84,006 8
3	6.2.3	0,225 g	weighing bottle	99,5 %	74,551 5
4	6.2.4	0,231 g	weighing bottle	99,0 %	228,222 0
5	6.2.5	0,311 g	weighing bottle	98,0 %	203,303 4
6	6.2.6	39 ml	graduated cylinder	—	—
7	6.2.7 ^c	0,292 g	weighing bottle	95,0 %	110,984 8
8	6.2.8	0,072 g	weighing bottle	99,0 %	142,042 8
9	6.2.9	6,118 g	weighing paper	99,0 %	121,135 6
10	6.2.6	0 ml to 5 ml	syringe dropper	—	—

^a The amounts of the reagents are changed depending upon their purities.

^b The purity given in this table is a typical purity for reagent available in most countries.

^c If calcium chloride dihydrate ($\text{CaCl}_2 \cdot 2\text{H}_2\text{O}$) is used, attention shall be given to the different molar weight:

– amount 0,371 g

– purity 99,0 %

– formula weight 147,015 2

6.3.2 Step 1

Put 700 ml of ion-exchanged and distilled water, with a stirring bar, into a 1 litre plastic beaker. Set it in the water bath ([4.2](#)) on the magnetic stirrer and cover it with a watch glass or plastic wrap. Heat the water in the beaker to $(36,5 \pm 1,5)^\circ\text{C}$ while stirring. [Annex A](#) shows an example of an apparatus for preparing the SBF.

6.3.3 Step 2

Dissolve the 1st to 8th reagents in the required order given in [Table 2](#) in the distilled water at $(36,5 \pm 1,5)^{\circ}\text{C}$, while considering the following.

- Glass containers should be avoided. A plastic container, with a smooth surface and without any scratches, is recommended, because apatite nucleation can be induced at the surface of a glass container or the edges of scratches.
- Dissolve a reagent only after the preceding one (if any) is completely dissolved.
- Dissolve the $\text{CaCl}_2/\text{CaCl}_2 \cdot 2 \text{H}_2\text{O}$ little by little as the reagent has a great effect on the precipitation of apatite.
- Rinse the graduated cylinder with 1 mol/l HCl before measuring the volume of 1 mol/l HCl.
- Measure the hygroscopic reagents such as $\text{K}_2\text{HPO}_4 \cdot 3 \text{H}_2\text{O}$, $\text{MgCl}_2 \cdot 6 \text{H}_2\text{O}$, $\text{CaCl}_2/\text{CaCl}_2 \cdot 2 \text{H}_2\text{O}$, KCl, Na_2SO_4 as quickly as possible.

6.3.4 Step 3

Insert the electrode of the pH meter ([4.3](#)) into the solution. Just before dissolving the TRIS, the pH of the solution should be $2,0 \pm 1,0$.

6.3.5 Step 4

Set the temperature of the solution at $(36,5 \pm 1,5)^{\circ}\text{C}$. If the amount of the solution is smaller than 0,9 l, add distilled water up to 0,9 l in total.

6.3.6 Step 5

With the solution temperature between $(36,5 \pm 1,5)^{\circ}\text{C}$, preferably $(36,5 \pm 0,5)^{\circ}\text{C}$, dissolve TRIS into the solution little by little, taking careful note of the pH change. After adding a small amount of TRIS, wait until the reagent is dissolved completely and the pH has become constant. Then add another small amount of TRIS.

It is recommended not to add a large amount of TRIS into the solution all at once, because the radical increase in local pH of the solution could lead to the precipitation of apatite. The following procedure is recommended: If the solution temperature is not within $(36,5 \pm 0,5)^{\circ}\text{C}$, add TRIS to raise the pH to $7,3 \pm 0,05$, then stop adding and wait for the solution temperature to reach $(36,5 \pm 0,5)^{\circ}\text{C}$. With the solution at $(36,5 \pm 0,5)^{\circ}\text{C}$, add more TRIS to raise the pH to under 7,45. The pH should not increase to over 7,45 at $(36,5 \pm 0,5)^{\circ}\text{C}$, taking account of the pH decrease with increasing solution temperature.

6.3.7 Step 6

Make sure that the temperature of the solution is maintained at $(36,5 \pm 0,5)^{\circ}\text{C}$. When the pH has risen to $7,45 \pm 0,01$, stop dissolving TRIS, then add HCl solution by syringe to lower the pH to $7,42 \pm 0,01$, taking care that the pH does not decrease below 7,40. After the pH has fallen to $7,42 \pm 0,01$, dissolve the remaining TRIS little by little until the pH has risen to $\leq 7,45$. If any TRIS remains, add the 1 mol/l -HCl and TRIS alternately into the solution. Repeat this process until the whole amount of TRIS is dissolved keeping the pH within the range of 7,42 to 7,45. After dissolving the whole amount of TRIS, adjust the temperature of the solution to $(36,5 \pm 0,2)^{\circ}\text{C}$. Adjust the pH of the solution by adding HCl solution little by little at a pH of $7,42 \pm 0,01$ at $(36,5^{\circ} \pm 0,2)^{\circ}\text{C}$ and then finally adjust it to 7,40 exactly at $36,5^{\circ}\text{C}$ on condition that the rate of solution temperature increase or decrease is less than $0,1^{\circ}\text{C}/\text{min}$.

6.3.8 Step 7

Remove the electrode of the pH meter from the solution, rinse it with distilled water and add the washings to the solution.

6.3.9 Step 8

Pour the pH-adjusted solution from the beaker into a 1 l volumetric flask. Rinse the surface of the beaker with distilled water several times and add the washings to the flask. Fix the stirring bar with a magnet to prevent it from falling into the volumetric flask.

6.3.10 Step 9

Add the distilled water up to the marked line (it is not necessary to adjust exactly, because the volume becomes smaller after cooling). Put a lid on the flask and close it using a plastic film.

6.3.11 Step 10

After mixing the solution in the flask, keep it in the water bath to cool it down to 20°C.

6.3.12 Step 11

After the solution temperature has fallen to 20°C, add distilled water up to the marked line.

6.4 Confirmation of ion concentration of SBF

Prepared SBF shall have the ion concentrations given in [Table 1](#). In order to confirm the ion concentrations of the SBF, chemical analysis of the SBF is recommended because SBF is a metastable solution supersaturated with respect to apatite.

It is also recommended that the apatite-forming ability of standard glasses in the prepared SBF be examined. Chemical compositions of the standard glasses for evaluating apatite-forming ability are shown in [Figure B.1](#). When standard glasses A, B and C for evaluating apatite-forming ability are soaked in SBF, an apatite layer should be detected by TF-XRD pattern after soaking for about 12 h, 24 h and 120 h.

6.5 Preservation of SBF

Prepared SBF should be preserved in a plastic bottle with a lid put on tightly and kept at $(7,5 \pm 2,5)^\circ\text{C}$ in a refrigerator. The SBF shall be used within 30 d of preparation.

It is recommended that the final product of SBF be sterilized by filtration to eliminate any dust particles and bacteria from the fluid, since dust can promote the heterogeneous nucleation of apatite and bacteria often phagocytose apatite formed in SBF. The sterilization should be carried out just after the preparation and/or just before evaluation for apatite-forming ability. For sterilization just after preparation (before preservation), the whole amount of as-prepared SBF is filtered by using a peristaltic pump through a sterile vented filter unit with a pore size of 0,22 μm at the flow rate of 85 ml/min to 100 ml/min. For sterilization just before starting evaluation for apatite-forming ability, the SBF is filtered by using a syringe attached with a sterile vented filter unit with a pore size of 0,22 μm . Either or both sterilization methods can be selected.

7 Procedure

7.1 For dense materials, measure the specimen dimensions to an accuracy of $\pm 0,1$ mm and calculate the surface area to an accuracy of 2 mm² for a thin plate.

7.2 Calculate the volume of SBF that is used for testing using Formula (1):

$$v_s = 100\text{mm} \cdot S_a \quad (1)$$

where


v_s is the volume of the SBF in mm^3 ;

S_a is the apparent surface area of the specimen in mm^2 .


For porous materials, the volume of SBF should be greater than the calculated v_s .

7.3 Put the calculated volume of SBF into a plastic bottle with a cap or beaker. After heating the SBF to $36,5^\circ\text{C}$ a specimen shall be placed in the SBF as shown in [Figure 2](#). The entire specimen shall be submerged in the SBF.

Pure, freshly prepared, dust-free SBF solution heated at 37°C for 4 weeks in a transparent bottle, even without any material for testing immersed in it, will precipitate apatite. If there happens to be a specimen immersed in that solution, those solution precipitates will then be deposited on the surface of the specimen. Therefore, it is recommended that the specimens be placed in the SBF as shown in [Figure 2 a\)](#) or [Figure 2 b\)](#). In case of placement as shown in [Figure 2 b\)](#), apatite formation should be examined on the lower surface of the specimen.



a) Disc



b) Rectangular

Figure 2 — Examples of specimens in SBF

7.4 After soaking in the SBF at $36,5^\circ\text{C}$ for different periods within four weeks, take out the specimen from the SBF and gently rinse it with distilled water.

A soaking time within four weeks is recommended.

The specimen shall then be dried in a desiccator without heating. A specimen, once taken out of SBF and dried, shall not be soaked again.

NOTE Bone bonding materials usually form apatite on their surfaces within four weeks.

7.5 Examine the surface of a specimen by TF-XRD and/or SEM until apatite is detected.

It is recommended to perform the TF-XRD measurement in the range of 3° to 50° in 2θ (θ) using $\text{CuK}\alpha$ ($\lambda = 0,154\ 05\ \text{nm}$) radiation as the source at a rate of $2^\circ/\text{min}$ and a 1° glancing angle against the incident beam on the specimen surface.

The dried specimen for SEM observation should be thinly metal-coated to induce electro conductivity. The SEM photos should be taken both at high magnifications (around $\times 10\,000$) and low magnifications (around $\times 1\,000$).

NOTE The TF-XRD measurement can clearly identify the apatite formation on the specimen. The SEM observation can observe the material formation on the specimen, but cannot identify whether apatite is formed or not. Therefore the SEM observation should be accompanied with the TF-XRD measurement. However, formed apatite grains and layers have characteristic features to be identified, and the apatite formation is sometimes estimated only on SEM.


8 Test report

The test report shall include the following information:

- a) all relevant material data including vintage, billet or component, specimen configurations and dimensions;
- b) specimen preparation procedure, including machining conditions for specimen surfaces;
- c) porosity of material as a percentage (optional);
- d) volume of SBF used in the measurement;
- e) soaking temperature of SBF ($^{\circ}\text{C}$);
- f) method of detecting the apatite on a specimen surface (TF-XRD and/or SEM);
- g) measurement conditions for TF-XRD with diffraction patterns and/or observation conditions for SEM with microphotographs showing the existence of apatite;
- h) presence or absence of apatite at each period; or estimated induction period (optional);
- i) number of specimens per condition;
- j) name of laboratory and date of the test;
- k) reference to this International Standard, i.e. ISO 23317:2014.

Annex A (informative)

Apparatus for preparing SBF

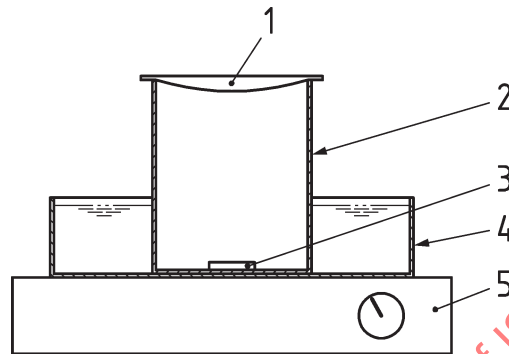**Key**

- 1 watch glass
- 2 polyethylene beaker
- 3 magnetic bar
- 4 water bath
- 5 magnetic stirrer

Figure A.1 — Example of apparatus for preparing SBF

Annex B (informative)


Preparation of standard glasses for evaluating apatite-forming ability

The compositions of the standard glasses are given in [Table B.1](#). The fine grade reagents of SiO_2 , Na_2CO_3 and CaCO_3 should be used to prepare standard glasses. See [Figure B.1](#).

Prepare the reagents in the amounts listed in [Table B.2](#), taking into consideration the mass loss after burning at selected temperatures. (Alternatively, it is desirable to use the pre-heated reagents in order to eliminate a mass loss; e.g. Na_2CO_3 , CaCO_3 and SiO_2 are pre-heated at 1 000°C for 10 h, 600°C for 2 h and 550°C for 1 h, respectively.)

After being measured, reagents are gathered in an alumina mortar and mechanically well mixed by use of a pestle for 30 min.

Powders (for glasses A, B and C) in a platinum crucible are melted at 1 400°C for 1,5 h and then poured out on to a stainless steel plate with spacers 2 mm thick set on the plate. The glass is pressed immediately with another stainless steel plate and formed into a plate 2 mm thick. The glass plates are then moved to another stainless steel plate pre-heated to 500 °C. After annealing, the glasses are cut into specimens under a non-aqueous cooling medium, polished with No. 400 abrasive paper and finally washed in acetone in an ultrasonic bath.

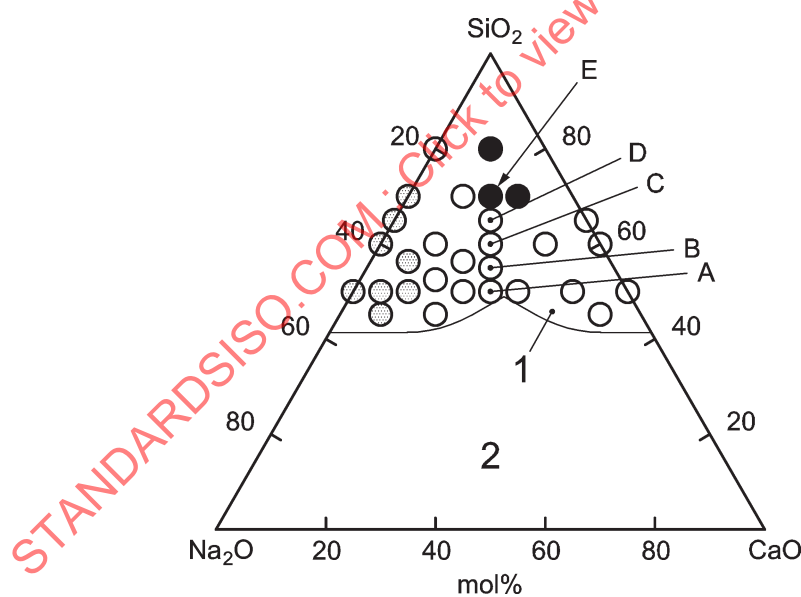

Key

- | | |
|---|----------------------|
| 1 | glass formation |
| 2 | no glass formation |
| ○ | apatite formation |
| ● | no apatite formation |
| ⊙ | dissolution |

Figure B.1 — Standard glasses in the Na_2O - CaO - SiO_2 system and apatite-forming ability after soaking in SBF for 30 d