

---

---

**Gas analysis — Preparation of calibration  
gas mixtures using dynamic volumetric  
methods —**

**Part 6:  
Critical orifices**

*Analyse des gaz — Préparation des mélanges de gaz pour étalonnage à  
l'aide de méthodes volumétriques dynamiques —*

*Partie 6: Orifices critiques*



**PDF disclaimer**

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.

STANDARDSISO.COM : Click to view the full PDF of ISO 6145-6:2003

© ISO 2003

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Case postale 56 • CH-1211 Geneva 20  
Tel. + 41 22 749 01 11  
Fax + 41 22 749 09 47  
E-mail [copyright@iso.org](mailto:copyright@iso.org)  
Web [www.iso.org](http://www.iso.org)

Published in Switzerland

## Contents

Page

|                              |                                                                               |           |
|------------------------------|-------------------------------------------------------------------------------|-----------|
| <b>1</b>                     | <b>Scope .....</b>                                                            | <b>1</b>  |
| <b>2</b>                     | <b>Normative references .....</b>                                             | <b>1</b>  |
| <b>3</b>                     | <b>Principle .....</b>                                                        | <b>1</b>  |
| <b>4</b>                     | <b>Application to preparation of gas mixtures .....</b>                       | <b>2</b>  |
| <b>4.1</b>                   | <b>Description of the orifice system and the experimental procedure .....</b> | <b>2</b>  |
| <b>4.2</b>                   | <b>Area of validity .....</b>                                                 | <b>4</b>  |
| <b>4.3</b>                   | <b>Operating conditions .....</b>                                             | <b>4</b>  |
| <b>5</b>                     | <b>Calculation of operating parameters and results .....</b>                  | <b>4</b>  |
| <b>5.1</b>                   | <b>Selection of suitable orifice systems .....</b>                            | <b>4</b>  |
| <b>5.2</b>                   | <b>Calculation of volume fraction .....</b>                                   | <b>5</b>  |
| <b>5.3</b>                   | <b>Sources of uncertainty .....</b>                                           | <b>5</b>  |
| <b>5.4</b>                   | <b>Uncertainty of volume fraction .....</b>                                   | <b>6</b>  |
| <b>Annex A (informative)</b> | <b>Premixed gases for preparation of mixtures of high dilution .....</b>      | <b>7</b>  |
| <b>Annex B (informative)</b> | <b>Practical hints .....</b>                                                  | <b>9</b>  |
| <b>Bibliography</b>          | <b>.....</b>                                                                  | <b>11</b> |

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 6145-6 was prepared by Technical Committee ISO/TC 158, *Analysis of gases*.

This second edition cancels and replaces the first edition (ISO 6145-6:1986), which has been technically revised.

ISO 6145 consists of the following parts, under the general title *Gas analysis — Preparation of calibration gas mixtures using dynamic volumetric methods*:

- *Part 1: Methods of calibration*
- *Part 2: Volumetric pumps*
- *Part 4: Continuous injection method*
- *Part 5: Capillary calibration devices*
- *Part 6: Critical orifices*
- *Part 7: Thermal mass-flow controllers*
- *Part 9: Saturation method*
- *Part 10: Permeation method*

Diffusion will be the subject of a future Part 8 to ISO 6145. Part 3 to ISO 6145, entitled *Periodic injections into a flowing gas*, has been withdrawn.

## Introduction

This part of ISO 6145 is one of a series of standards that present various dynamic volumetric methods used for the preparation of calibration gas mixtures.

STANDARDSISO.COM : Click to view the full PDF of ISO 6145-6:2003

STANDARDSISO.COM : Click to view the full PDF of ISO 6145-6:2003

# Gas analysis — Preparation of calibration gas mixtures using dynamic volumetric methods —

## Part 6: Critical orifices

### 1 Scope

This part of ISO 6145 specifies a method for the continuous production of calibration gas mixtures, containing two or more components, from pure gases or other gas mixtures by use of critical orifice systems. By selection of appropriate combinations of orifices and with the use of pure gases, the volume fraction of the calibration component in the calibration gas mixture can be varied by a factor of  $10^4$ . Additionally, it can be changed by a factor of  $10^2$  by changing the initial pressures in the orifice systems. The uncertainty of the method depends mainly upon the flow calibration method and the variations in temperature and outlet pressure. The relative expanded uncertainty in the volume fraction obtainable for a binary mixture (at a coverage factor of 2) is 3 %.

If pre-mixed gases are used instead of pure gases, much lower volume fractions can be obtained (see Annex A). The mass flow rates or volume flow rates, from which the mass or volume fractions are determined, can be calculated and can be independently measured by a suitable method given in ISO 6145-1.

The merits of the method are that multi-component mixtures can be prepared as readily as binary mixtures if the appropriate number of orifices is utilized, and that a large quantity of calibration gas mixture can be prepared on a continuous basis. The range of flow rates can be from several millilitres per minute to approximately 10 l/min.

Although particularly applicable to preparation of gas mixtures at barometric pressure, the method also provides a means of preparation of calibration gas mixtures at pressures above barometric pressure.

Annex B gives practical hints on the use of the method.

### 2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 6143, *Gas analysis — Comparison methods for determining and checking the composition of calibration gas mixtures*

ISO 6145-1, *Gas analysis — Preparation of calibration gas mixtures using dynamic volumetric methods — Part 1: Methods of calibration*

### 3 Principle

When passed through a critical orifice at increasing upstream pressure  $p_1$ , the volume flow rate of gas passing through the orifice will increase. When the ratio of the gas pressure upstream  $p_1$  and the gas pressure downstream of the orifice  $p_2$  has reached a critical value, on further increase of  $p_1$  the volume flow rate of the gas becomes independent with respect to  $p_2$ .

For a given gas, and at constant temperature the critical pressure ratio is:

$$\left(\frac{p_2}{p_1}\right)_{\text{crit}} = \left(\frac{2}{\gamma + 1}\right)^{\frac{\gamma}{\gamma - 1}} \quad (1)$$

where  $\gamma$  is the ratio of the molar heat capacities of the gas at constant pressure and at constant volume.

For monatomic, diatomic and triatomic gases, this critical pressure ratio is approximately 0,5.

Orifice systems which are operated at pressure ratios  $p_2/p_1$  less than  $(p_2/p_1)_{\text{crit}}$  are termed "critical orifices". Use of such systems provides a means of maintaining constant flow rates of gases. In actual practice it is convenient to arrange the system so that  $p_2$  is equal to the prevailing barometric pressure.

To prepare calibration gas mixtures, the complementary gas is supplied at known flow rate, from a critical orifice, to meet the calibration component emerging from another critical orifice. The mixture is then allowed to pass along a mixing tube, at the end of which the flow rate is measured by a suitable method as given in ISO 6145-1. Since the volume flow rate of the calibration component remains the same whether or not the complementary gas is flowing, it can be measured after the flow of complementary gas has been stopped. The concentration of the calibration gas mixture is calculated from the two measured critical flow rates.

## 4 Application to preparation of gas mixtures

### 4.1 Description of the orifice system and the experimental procedure


A schematic diagram of the arrangement for preparation of binary mixtures is shown in Figure 1.

In Figure 1, the orifices 9 and 10, respectively, for the complementary gas and the calibration component to be added are mounted in the orifice system (11). Cylinders 1 and 13, respectively, contain the complementary gas and the other gaseous component, and are connected to the mixing system via pressure-reducing valves (3 and 15) and metallic filters (5 and 17), which provide protection against contamination. In each of the lines, and upstream of the filters, are a pressure-reducing valve and a pressure gauge. A shut-off valve (8) is provided in the complementary gas line and a venting valve is included in the other line.

To operate the gas-mixing system, the valves of the gas cylinders are opened and the readings on the pressure gauges 4 and 16 are adjusted, each to a value approximately 200 kPa (2 bar) above the values anticipated at pressure gauges 7 and 20 respectively.

The pressure regulators (6 and 18) are opened so that the complementary gas and the calibration component flow through the respective orifices. The flow of complementary gas is then stopped by closing the shut-off valve 8. The other line is then flushed with the calibration component by repeated opening and closure of the venting valve 19. Valve 19 is then closed and pressure regulator 18 is adjusted so as to set the pressure at gauge 20 to the value necessary to produce the required flow rate (see below). The flow rate is then measured, by one of the methods given in ISO 6145-1, at outlet 12 of the orifice system (11).

The shut-off valve 8 is then opened and pressure regulator 6 is adjusted to set the pressure indicated on pressure gauge 7 to the value necessary to produce the required flow rate. The combined flow rates of the complementary gas and the calibration component are then measured by a suitable method according to ISO 6145-1.

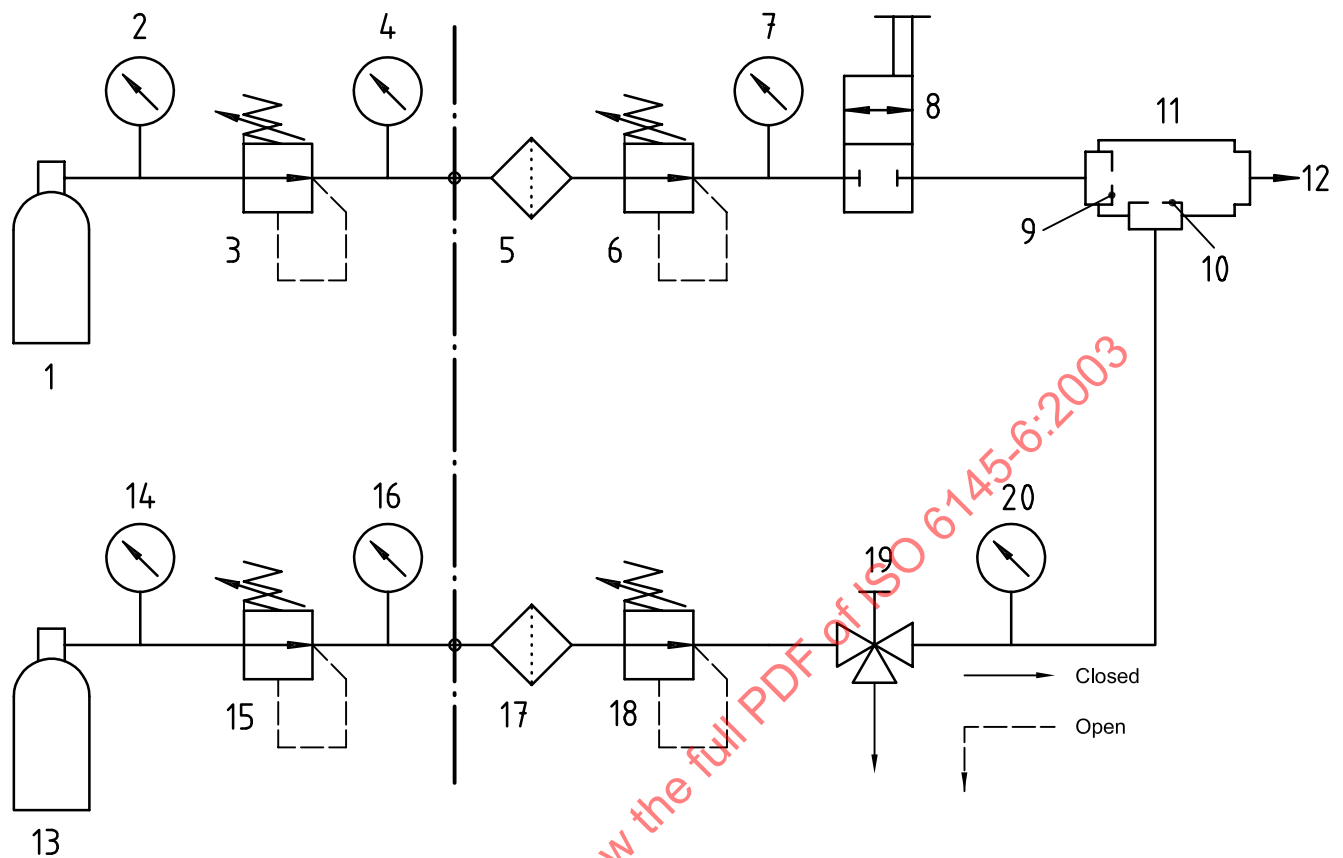

### Key

- 1 pressure cylinder (complementary gas)
- 2 pressure gauge (inlet pressure)
- 3 pressure-reducing valve
- 4 pressure gauge (delivery pressure)
- 5 filter
- 6 pressure regulator
- 7 pressure gauge
- 8 shut-off valve
- 9 orifice (complementary gas)
- 10 orifice (calibration component)
- 11 orifice system
- 12 exit for calibration gas mixture
- 13 pressure cylinder (calibration component)
- 14 pressure gauge (inlet pressure)
- 15 pressure-reducing valve
- 16 pressure gauge (delivery pressure)
- 17 filter
- 18 pressure regulator
- 19 vent valve
- 20 pressure gauge

**Figure 1 — Preparation of calibration gas mixtures with a critical orifice system**

## 4.2 Area of validity

The method is applicable to preparation of mixtures of non-reacting species, i.e. those which do not react with any material of construction of the flow path within the orifice system or the ancillary equipment. Particular care shall be exercised if the method is considered as a means of preparation of gaseous mixtures that contain components which form potentially explosive mixtures in air. Steps shall be taken to ensure that the apparatus is safe, for example by means of in-line flame arrestors in addition to the items listed in 4.1 (unless the in-line metallic filters already present are in fact approved sintered metal flame arrestors). This is of particular importance in this method because the gases in the dilution system are at pressures appreciably above the prevailing barometric pressure.

The method is not absolute and each orifice system shall be calibrated for the particular gas for which it is to be used. This is necessary because the formula for the volume flow rate of a gas includes the molar mass.

## 4.3 Operating conditions

The general precautions common to all dynamic techniques of preparation shall be observed. It is essential that attention is paid to the materials used in construction of the flow system. Only materials of low porosity and which are non-adsorbing are suitable. The pipe work shall be clean and all joints secure.

## 5 Calculation of operating parameters and results

### 5.1 Selection of suitable orifice systems

The volume flow rate of a gas through an orifice at  $p_2 \leq 0,5p_1$  is given by:

$$q_0 = \frac{p_1}{p_n} \sqrt{\frac{T_n}{T_1}} \cdot A \sqrt{\frac{RT_n}{M}} \cdot \sqrt{\gamma \left( \frac{2}{\gamma + 1} \right)^{\frac{\gamma+1}{\gamma-1}}} \quad (2)$$

where (in the appropriate units)

$q_0$  is the volume flow rate of the gas under normal conditions;

$p_n$  is the standard atmospheric pressure (101,325 kPa);

$T_n$  is the normal temperature (273,15 K);

$p_1$  is the pressure of the gas upstream of the orifice;

$T_1$  is the upstream temperature of the gas;

$R$  is the universal gas constant [8,314 510 J/(mol·K)];

$M$  is the molar mass of the gas, in grams per mole;

$\gamma$  is the ratio of the molar heat capacities of the gas at constant pressure and at constant volume;

$A$  is the cross-sectional area of the orifice;

$p_2$  is the pressure of the gas downstream of the orifice.

At a constant temperature,  $T_1$ , Equation (2) can be simplified to:

$$q_0 = D \cdot d^2 \cdot M^{-\frac{1}{2}} \cdot p_1 \quad (3)$$

where

$d$  is the diameter of the orifice;

$D$  is a constant.

For polyatomic gaseous molecules, the ratio of the molar heat capacities,  $\gamma$ , is calculated from the known value of  $C_p$ , the molar heat capacity at constant pressure, and the value of  $C_V$ , the molar heat capacity at constant volume calculated from the relationship  $C_p - C_V = R$ . The value for  $D$  can then be calculated.

When the constant multiplier has been evaluated, Equation (3) is applied to calculate the diameter of the orifice to deliver the required flow rate of a gas of molar mass,  $M$ , at upstream pressure  $p_1$ .

## 5.2 Calculation of volume fraction

The volume fraction,  $\varphi_A$ , in the calibration gas mixture, is calculated from the equation:

$$\varphi_A = q_A / (q_A + q_B) \quad (4)$$

in which  $q_A$  and  $q_B$  are the volume flow rates of the calibration component and the complementary gas, respectively.

When the flow rates are determined with reference to ISO 6145-1, due consideration shall be given to the uncertainty associated with the method selected.

## 5.3 Sources of uncertainty

### 5.3.1 General

The volume flow rate of a gas through an orifice depends on the pressure upstream from the orifice and the temperature at the orifice. It is essential, therefore, to use good-quality pressure-reducing valves and pressure regulators in order to maintain the upstream pressure at a constant value. The coefficient of expansion of the calibration component and that of the complementary gas will differ slightly, depending upon the respective degrees of departure from ideality. However, to a very good approximation, small changes in temperature will cause negligible change in the flow rate ratio, provided that the temperature is the same at each orifice.

### 5.3.2 Downstream pressure

The thermodynamic treatment, which leads to the independence of the volumetric flow rate with respect to the downstream pressure, is not completely realized in actual practice, i.e. in the case of real orifices. At supercritical flow, therefore, the downstream pressure ( $p_2$ ) still has some influence that can result in changes in volumetric flow rate if fluctuations in  $p_2$  occur. The characteristic curve relating flow rate to pressure depends on the geometry of the orifice and the flow direction through the orifice. For measurements of the highest accuracy, this curve shall be established by calibration.

### 5.3.3 Temperature differentials

The orifice system would normally be arranged so that the temperature at each orifice is identical. However, if there is a temperature difference between the two components to produce a binary mixture, the volume flow rate of one shall be corrected by application of the coefficient of thermal expansion of the gas. For an ideal gas the coefficient is 0,003 661 per kelvin, and this value can be applied for real gases to a very good approximation for small differences in temperature between the gaseous components.

The following example demonstrates the magnitude of the errors which may be involved. The coefficient of thermal expansion of carbon dioxide is 0,003 72 per kelvin; that of hydrogen is 0,003 66 per kelvin. The method is employed to prepare a mixture of hydrogen and carbon dioxide at 293 K in which the volume fractions are to

be 0,5. However, there is a temperature differential such that the hydrogen is at 292 K and the carbon dioxide is at 294 K. The volume fraction of hydrogen in the mixture at 293 K is  $1,003\,66 \times 0,5 = 0,502$  and that of carbon dioxide is  $(1 - 0,003\,72) \times 0,5 = 0,498$ . The error in the volume fraction for a 2 K temperature differential is therefore 0,4 % relative. This demonstrates that it is necessary to maintain the component gases at the same temperature as each other or to apply corrections to the volume flow rates if there is a temperature differential.

#### 5.3.4 Inefficient mixing

Another possible source of error is inefficient mixing of the calibration component and the complementary gas. A check of the efficiency of mixing is provided by verification of the volume (or mass) fraction by means of the comparison method (see ISO 6143).

### 5.4 Uncertainty of volume fraction

The uncertainty of the volume fraction of the calibration component in the calibration mixture, at constant temperature and pressure, can be estimated from the separate uncertainties in the flow rates of the calibration component and the complementary gas.

The volume fraction of component A is given by Equation (4).

The relative expanded uncertainty in  $\varphi_A$  is then given by:

$$\frac{U(\varphi_A)}{\varphi_A} = \left[ \frac{2q_B}{q_A + q_B} \right] \left[ \left( \frac{u(q_A)}{q_A} \right)^2 + \left( \frac{u(q_B)}{q_B} \right)^2 \right]^{\frac{1}{2}} \quad (5)$$

The derivation of this formula is presented in Annex C of ISO 6145-7:2001<sup>[1]</sup>. The r.m.s. sum of the relative standard uncertainty contributions is multiplied by the coverage factor  $k = 2$  to give a coverage probability of approximately 95 %.

The standard uncertainties  $u(q_A)$  and  $u(q_B)$  in the respective flow rates are obtained by reference to ISO 6145-1 for the selected method of flow calibration.

This estimate of the relative uncertainty in the composition rests entirely on the uncertainties in measurements of flow rates. The other factor to be taken into account is the efficiency of mixing. To check the effectiveness of a mixing system to provide a homogeneous calibration gas mixture, mixtures shall be prepared by the method as described and the compositions shall be checked by the comparison method of ISO 6143. This procedure also identifies bias from other sources and establishes traceability against standard mixtures.

## Annex A (informative)

### Premixed gases for preparation of mixtures of high dilution

#### A.1 Calculation of results

If premixed gases are used instead of pure gases, mixtures of higher dilution can be prepared. Calculation of results is then as follows.

The volume fraction of component A in the final calibration gas mixture is given by:

$$\begin{aligned}\varphi_A &= \frac{\varphi'_A q_M + \varphi''_A q_B}{q_M + q_B} \\ &= \frac{\varphi'_A q_M + \varphi''_A q_B}{q_\varphi}\end{aligned}\quad (\text{A.1})$$

where

- $\varphi'_A$  is the volume fraction of A in the premixed gas;
- $\varphi''_A$  is the volume fraction of A in the complementary gas B (this will normally be zero);
- $q_M$  is the volume flow rate of the premixed gas;
- $q_B$  is the volume flow rate of the complementary gas B;
- $q_\varphi$  is the volume flow rate of the calibration gas mixture.

NOTE  $q_\varphi = q_M + q_B$  only if there is no volume change on mixing.

#### A.2 Uncertainty of volume fraction

It is necessary to take into account the uncertainties of the volume flow rates and the uncertainties of the volume fractions of the component in the premixed gas and also in the complementary gas (if relevant). Normally the complementary gas will not contain the calibration component.

For the case in which the complementary gas does not contain the calibration component A:

$$\varphi_A = \frac{\varphi'_A q_M}{q_M + q_B} \quad (\text{A.2})$$

and the relative expanded uncertainty in the volume fraction ( $\varphi_A$ ) is given by:

$$\frac{U(\varphi_A)}{\varphi_A} = \frac{2q_B}{q_B + q_M} \left[ \left( \frac{u(q_M)}{q_M} \right)^2 + \left( \frac{u(q_B)}{q_B} \right)^2 + \left( \frac{q_M + q_B}{q_B} \right)^2 \left( \frac{u(\varphi'_A)}{\varphi'_A} \right)^2 \right]^{\frac{1}{2}} \quad (\text{A.3})$$

The derivation of this formula is presented in Annex C of ISO 6145-7:2001<sup>[4]</sup>. The r.m.s. sum of the standard uncertainty contributions is multiplied by the coverage factor  $k = 2$  to give a coverage probability of approximately 95 %.

The uncertainties in all of the flow rates are obtained with reference to ISO 6145-1 for the selected method of flow calibration.

STANDARDSISO.COM : Click to view the full PDF of ISO 6145-6:2003