
**Stainless steel needle tubing for the
manufacture of medical devices —
Requirements and test methods**

*Tubes d'aiguilles en acier inoxydable pour la fabrication de matériel
médical — Exigences et méthodes d'essai*

STANDARDSISO.COM : Click to view the full PDF of ISO 9626:2016



STANDARDSISO.COM : Click to view the full PDF of ISO 9626:2016



COPYRIGHT PROTECTED DOCUMENT

© ISO 2016, Published in Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Ch. de Blandonnet 8 • CP 401
CH-1214 Vernier, Geneva, Switzerland
Tel. +41 22 749 01 11
Fax +41 22 749 09 47
copyright@iso.org
www.iso.org

Contents

Page

Foreword	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Materials	2
5 Requirements	2
5.1 General.....	2
5.2 Surface finish and visual appearance.....	2
5.3 Cleanliness.....	2
5.4 Limits for acidity and alkalinity.....	2
5.5 Size designation.....	2
5.6 Dimensions.....	2
5.7 Sample size.....	5
5.8 Stiffness.....	5
5.9 Resistance to breakage.....	7
5.10 Resistance to corrosion.....	7
Annex A (normative) Methods for preparation of extracts	8
Annex B (normative) Test method for stiffness of tubing	9
Annex C (normative) Test method for resistance of tubing to breakage	11
Annex D (normative) Test method for resistance to corrosion	13
Annex E (informative) Rationale with respect to test method for stiffness of tubing	14
Bibliography	23

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT) see the following URL: [Foreword - Supplementary information](#).

The committee responsible for this document is ISO/TC 84, *Devices for administration of medicinal products and catheters*.

This second edition cancels and replaces the first edition (ISO 9626:1991), which has been technically revised. It also incorporates the Amendment ISO 9626:1991/Amd 1:2001.

The main changes to the previous edition of ISO 9626 introduced by this revision are the following:

- a) addition of specifications for stainless steel needle tubing for metric sizes 0,18 mm, 0,2 mm, 0,23 mm and 0,25 mm and to reflect the introduction of thinner tubing to allow greater comfort when injecting, particularly for infants and in paediatric use;
- b) addition of wall thickness designations beyond regular-walled and thin-walled tubing;
- c) addition of minimum inner diameters for additional items where possible;
- d) revision of the means of specifying the steels to be used;
- e) revision of the table of tubing dimensions and stiffness parameters.

[Annex A](#), [Annex B](#), [Annex C](#), [Annex D](#) and [Annex E](#) form an integral part of this International Standard.

Introduction

Guidance on transition periods for implementing the requirements of this International Standard is given in ISO/TR 19244.

STANDARDSISO.COM : Click to view the full PDF of ISO 9626:2016

[STANDARDSISO.COM](https://standardsiso.com) : Click to view the full PDF of ISO 9626:2016

Stainless steel needle tubing for the manufacture of medical devices — Requirements and test methods

1 Scope

This International Standard applies to rigid stainless steel needle tubing suitable for use in the manufacture of hypodermic needles and other medical devices primarily for human use.

This International Standard provides requirements and test methods for the tubes manufactured for needles as component used in medical devices. Additional performance testing on the tube aspect may be required when the component is incorporated in the ready-to-use device.

This International Standard specifies the dimensions and mechanical properties of steel tubing of designated metric sizes 3,4 mm (10 Gauge) to 0,18 mm (34 Gauge).

It does not apply to flexible stainless steel tubing because the mechanical properties differ from those specified for rigid tubing in this International Standard. However, manufacturers and purchasers of flexible tubing are encouraged to adopt the dimensional specifications given in this International Standard.

2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 3696, *Water for analytical laboratory use — Specification and test methods*

ISO 15510, *Stainless steels — Chemical composition*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

3.1

designated metric size

outer diameter designation of the tubing as defined in [Table 1](#)

Note 1 to entry: It is expressed in millimetres.

3.2

gauge

legacy size designation

Note 1 to entry: A particular gauge size corresponds to a designated metric size defining limits for outer diameters.

3.3

wall thickness

material thickness between the inner and outer diameter of the tube

Note 1 to entry: It is expressed as RW=Regular Wall, TW=Thin Wall, ETW= Extra Thin Wall, and UTW=Ultra Thin Wall as designated in [Table 1](#).

4 Materials

Tubing shall be made of stainless steels listed in ISO 15510. The chosen materials shall be in accordance with the requirements indicated in this International Standard. Selection of specific stainless steel material shall be made in consideration with the intended use, e.g. long-term contact with drugs and should consider biocompatibility requirements.

NOTE Suitable biocompatibility requirements can be found in ISO 10993-1.

5 Requirements

5.1 General

For the selection of tubing for a specific application and intended use, a risk based approach shall be applied.

5.2 Surface finish and visual appearance

When examined by normal or corrected vision, the outside surface of the tubing shall be smooth and free from defects.

Surface finish specifications may be different based on the final function of the medical device; in such cases, the medical device manufacturer should prepare specific specifications for surface finishing.

When examined by normal or corrected vision, the needle tube shall appear straight and of regular roundness.

5.3 Cleanliness

When examined by normal or corrected vision, the surfaces of the tubing shall be free from metal soil and processing agents.

Cleanliness specifications may be different based on the final function of the medical device; in such cases, the medical device manufacturer should prepare specific specifications for cleanliness.

5.4 Limits for acidity and alkalinity

When determined with a laboratory pH meter and using a general purpose electrode, the pH value of an extract prepared in accordance with [Annex A](#) shall be within one pH unit of that of the control fluid.

5.5 Size designation

Tubing size shall be designated by the nominal outer diameter, expressed in millimetres (i.e. the designated metric size), corresponding gauge size (e.g. G31 or 31G), and by wall thickness.

EXAMPLE 0,25 mm (31G) ETW.

5.6 Dimensions

The dimensions of tubing shall be as given in [Table 1](#).

Table 1 — Dimensions of tubing

Designated metric size mm	Gauge	OD _{MIN} mm	OD _{MAX} mm	Wall	ID _{MIN} mm
0,18	34	0,178	0,191	RW	0,064
				TW	0,091
				ETW	0,105
0,20	33	0,203	0,216	RW	0,089
				TW	0,105
				ETW	0,125
0,23	32	0,229	0,241	RW	0,089
				TW	0,105
				ETW	0,125
				UTW	0,146
0,25	31	0,254	0,267	RW	0,114
				TW	0,125
				ETW	0,146
				UTW	0,176
0,30	30	0,298	0,320	RW	0,133
				TW	0,165
				ETW	0,190
				UTW	0,240
0,33	29	0,324	0,351	RW	0,133
				TW	0,190
				ETW	0,240
				UTW	0,265
0,36	28	0,349	0,370	RW	0,133
				TW	0,190
0,40	27	0,400	0,420	RW	0,184
				TW	0,241
0,45	26	0,440	0,470	RW	0,232
				TW	0,292
0,50	25	0,500	0,530	RW	0,232
				TW	0,292
0,55	24	0,550	0,580	RW	0,280
				TW	0,343
0,60	23	0,600	0,673	RW	0,317
				TW	0,370
				ETW	0,460
NOTE 1 RW = Regular Wall; TW = Thin Wall; ETW = Extra Thin Wall; UTW = Ultra Thin Wall.					
NOTE 2 Needle sizes below 0,25 mm, consideration can be made to the measurement uncertainty of existing measurement equipment.					
NOTE 3 This International Standard does not specify maximum inner diameter.					
NOTE 4 OD = outer diameter; ID = inner diameter.					

Table 1 (continued)

Designated metric size mm	Gauge	OD _{MIN} mm	OD _{MAX} mm	Wall	ID _{MIN} mm
0,70	22	0,698	0,730	RW	0,390
				TW	0,440
				ETW	0,522
0,80	21	0,800	0,830	RW	0,490
				TW	0,547
				ETW	0,610
				UTW	0,645
0,90	20	0,860	0,920	RW	0,560
				TW	0,635
				ETW	0,687
				UTW	0,713
1,10	19	1,030	1,100	RW	0,648
				TW	0,750
				ETW	0,850
				UTW	0,891
1,20	18	1,200	1,300	RW	0,790
				TW	0,910
				ETW	1,041
1,40	17	1,400	1,510	RW	0,950
				TW	1,156
				ETW	1,244
				UTW	1,276
1,60	16	1,600	1,690	RW	1,100
				TW	1,283
				ETW	1,390
1,80	15	1,750	1,900	RW	1,300
				TW	1,460
				ETW	1,560
2,10	14	1,950	2,150	RW	1,500
				TW	1,600
				ETW	1,727
2,40	13	2,300	2,500	RW	1,700
				TW	1,956
2,70	12	2,650	2,850	RW	1,950
				TW	2,235
NOTE 1 RW = Regular Wall; TW = Thin Wall; ETW = Extra Thin Wall; UTW = Ultra Thin Wall.					
NOTE 2 Needle sizes below 0,25 mm, consideration can be made to the measurement uncertainty of existing measurement equipment.					
NOTE 3 This International Standard does not specify maximum inner diameter.					
NOTE 4 OD = outer diameter; ID = inner diameter.					

Table 1 (continued)

Designated metric size mm	Gauge	OD _{MIN} mm	OD _{MAX} mm	Wall	ID _{MIN} mm
3,00	11	2,950	3,150	RW	2,200
				TW	2,464
3,40	10	3,300	3,500	RW	2,500
				TW	2,819
NOTE 1 RW = Regular Wall; TW = Thin Wall; ETW = Extra Thin Wall; UTW = Ultra Thin Wall.					
NOTE 2 Needle sizes below 0,25 mm, consideration can be made to the measurement uncertainty of existing measurement equipment.					
NOTE 3 This International Standard does not specify maximum inner diameter.					
NOTE 4 OD = outer diameter; ID = inner diameter.					

5.7 Sample size

Where sampling is applicable, the sample sizes shall be determined on the basis of risk assessment principles and be included in the tube specification and based on the intended use.

5.8 Stiffness

When tested in accordance with [Annex B](#), the tubing shall show a deflection not greater than the relevant value given in [Table 2](#).

For tubes where stiffness test parameters are not defined in this International Standard, the medical device manufacturer shall prepare specific stiffness requirements based on a risk assessment of the final intended use of the tube.

Consideration should be given to the final product intended use of the tube to determine if additional tests are required.

Table 2 — Conditions for stiffness test

Designated metric size	Regular-walled tubing			Thin-walled tubing			Extra-thin walled tubing			Ultra-thin walled tubing		
	Span mm ± 0,1	Bending force N ± 0,1	Maximum deflection mm	Span mm ± 0,1	Bending force N ± 0,1	Maximum deflection mm	Span mm ± 0,1	Bending force N ± 0,1	Maximum deflection mm	Span mm ± 0,1	Bending force N ± 0,1	Maximum deflection mm
0,18	a	a	a	a	a	a	a	a	a	a	a	a
0,2	5,0	0,6	0,25	5,0	0,6	0,27	a	a	a	a	a	a
0,23	5,0	0,9	0,20	5,0	0,9	0,20	5,0	0,9	0,22	5,0	0,9	0,25
0,25	5,0	1,1	0,17	5,0	1,1	0,18	5,0	1,1	0,21	5,0	1,1	0,24
0,3	5,0	1,3	0,11	5,0	1,3	0,11	5,0	1,3	0,16	5,0	1,3	0,20
0,33	5,0	1,6	0,09	5,0	1,6	0,12	5,0	1,6	0,17	5,0	1,6	0,19
0,36	5,0	3,6	0,14	5,0	3,6	0,14	a	a	a	a	a	a
0,4	9,5	2,7	0,52	7,5	3,4	0,34	a	a	a	a	a	a
0,45	10,0	3,1	0,45	10,0	3,1	0,51	a	a	a	a	a	a
0,5	10,0	5,1	0,37	10,0	5,1	0,40	a	a	a	a	a	a
0,55	10,0	6,4	0,34	10,0	6,4	0,36	a	a	a	a	a	a
0,6	12,5	4,8	0,33	12,5	4,8	0,43	12,5	4,8	0,51	a	a	a
0,7	15,0	6,7	0,42	15,0	6,7	0,52	15,0	6,7	0,60	a	a	a
0,8	15,0	9,6	0,38	15,0	9,6	0,45	15,0	9,6	0,51	a	a	a
0,9	17,5	9,0	0,48	17,5	9,0	0,56	17,5	9,0	0,60	a	a	a
1,1	25,0	9,7	0,71	25,0	9,7	0,97	25,0	9,7	1,08	a	a	a
1,2	25,0	12,2	0,51	25,0	12,2	0,81	a	a	a	a	a	a
1,4	25,0	16,6	0,46	25,0	16,6	0,68	25,0	16,6	0,82	a	a	a
1,6	25,0	22,0	0,25	25,0	22,0	0,30	25,0	22,0	0,34	a	a	a
1,8	25,0	25,0	0,35	25,0	25,0	0,45	a	a	a	a	a	a
2,1	30,0	40,0	0,40	30,0	40,0	0,50	a	a	a	a	a	a
2,4	40,0	40,0	0,38	40,0	40,0	0,65	a	a	a	a	a	a
2,7	40,0	50,0	0,31	40,0	50,0	0,45	a	a	a	a	a	a
3	50,0	50,0	0,41	50,0	50,0	0,55	a	a	a	a	a	a
3,4	50,0	60,0	0,32	50,0	60,0	0,46	a	a	a	a	a	a
a	No data are available; therefore, this International Standard does not specify stiffness properties for these sizes of tubing.											

5.9 Resistance to breakage

When tested in accordance with [Annex C](#), the tubing shall not show visible breakage when examined by normal or corrected vision.

NOTE Consideration can be given to the final product's intended use to determine if additional tests are warranted.

5.10 Resistance to corrosion

When tested in accordance with [Annex D](#), the immersed half of the tubing shall show no evidence of corrosion resulting from the test.

NOTE Consideration can be given to the final product's intended use to determine if additional tests are warranted, e.g. long term drug product contact.

STANDARDSISO.COM : Click to view the full PDF of ISO 9626:2016

Annex A (normative)

Methods for preparation of extracts

A.1 Principle

The stainless steel tubing is immersed in water in order to extract soluble components.

A.2 Apparatus and reagents

A.2.1 Freshly distilled or deionized water, of grade 3 in accordance with ISO 3696.

A.2.2 Selection of laboratory borosilicate glassware.

A.3 Procedure

A.3.1 Immerse 3 g of tubing in 250 ml of water ([A.2.1](#)) in a suitable container made from borosilicate glass ([A.2.2](#)). Ensure that the surface of the stainless tubing, including the inside of the tubing, is in contact with the water.

Maintain the water at a temperature of $(37 + \frac{3}{0})$ °C for (60 ± 2) min. Remove the tubing and ensure that all water from the inside and outside surfaces of the tubing are returned to the container.

A.3.2 Prepare the control fluid by following the procedure given in [A.3.1](#) but omitting the tubing.

Annex B (normative)

Test method for stiffness of tubing

B.1 Principle


A specified force is applied to the centre of the specified length of tubing, which is supported at both ends, and the amount of deflection measured.

B.2 Apparatus

B.2.1 Stiffness testing apparatus, capable of applying a force of up to 60 N downwards normal to the tubing with an accuracy of $\pm 0,1$ N, by means of a plunger having a lower end in the form of a blunt wedge formed by two plane surfaces inclined at 60° to one another and a cylindrical surface of radius of 1 mm and length at least 5 mm.

An example of a suitable apparatus is illustrated in [Figure B.1](#).

B.2.2 Equipment, capable of measuring the deflection of the tubing to the nearest 0,01 mm.

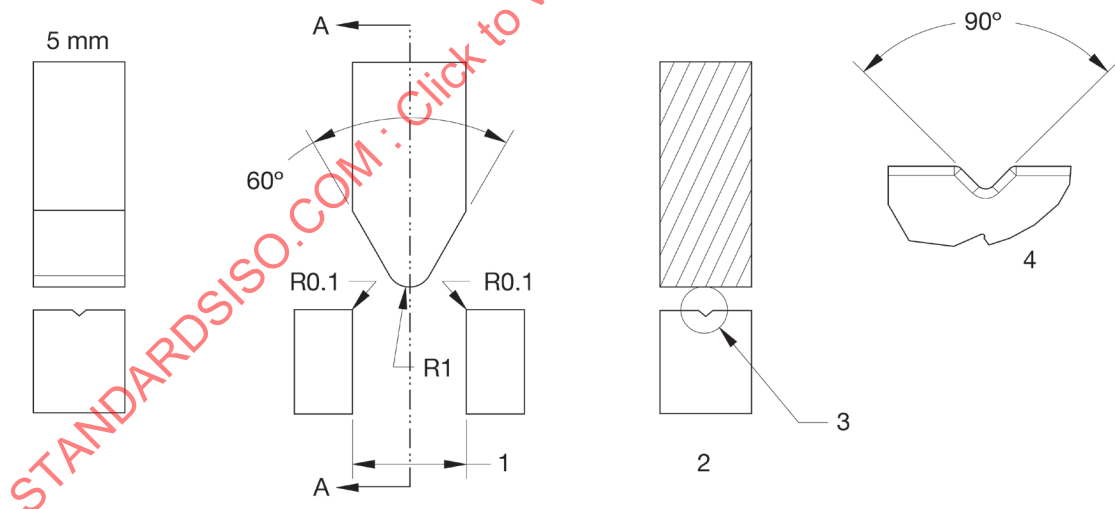

Key

- 1 span
- 2 section A-A
- 3 see detail 4
- 4 detail

Figure B.1 — Apparatus for stiffness test

B.3 Procedure

B.3.1 Place the tubing on the stiffness testing apparatus ([B.2.1](#)) and adjust the tubing and the stiffness testing apparatus so that

- a) span is as given in [Table 2](#) for the designated metric size of the tubing,
- b) the bottom surface of the plunger is at the centre of the span, and
- c) the tubing is normal to the supporting members and the loading plunger, and the centre of the tubing is at the centre of the span.

B.3.2 Apply a downward force given in [Table 2](#) for the designated metric size of the tubing at a speed between 1 mm/min and 10 mm/min.

B.3.3 Measure and record ([B.2.2](#)) to the nearest 0,01 mm the deflection of the tubing at the point of application of the force.

B.4 Test report

The test report shall contain at least the following information:

- a) the identity and designated metric size of the tubing;
- b) whether the tubing was of RW, TW, ETW or UTW type;
- c) the measured deflection, expressed in millimetres to the nearest 0,01 mm;
- d) the date of testing;
- e) the type of stainless steel alloy used, chosen according to [Clause 4](#).

Annex C (normative)

Test method for resistance of tubing to breakage

C.1 Principle

One end of the tubing is firmly fixed and a force applied to the tubing at a specified distance from the point of fixation, so as to bend the tubing through a specified angle, first in one direction and then in the opposite direction, for a specified number of cycles.

C.2 Apparatus

C.2.1 Support and device for fixing the tubing.

C.2.2 Equipment, capable of applying a force to the tubing sufficient to bend it through an angle of up to 25°.

C.3 Procedure

C.3.1 Rigidly fix one end of the tubing in the support ([C.2.1](#)).

C.3.2 Apply ([C.2.2](#)), at the distance given in [Table C.1](#), a force of sufficient magnitude to cause the tubing to bend in one plane through an angle of $(25 \pm 1)^\circ$ for regular-walled tubing, $(20 \pm 1)^\circ$ for thin-walled tubing, or $(15 \pm 1)^\circ$ for extra-thin-walled and ultra-thin walled tubing.

C.3.3 Apply the force in the reverse direction so as to cause the tubing to bend through the same angle in the reverse direction.

C.3.4 Perform 20 complete cycles of reversal of force at a rate of 0,5 Hz and examine the tubing visually for breakage.

C.4 Test report

The test report shall contain at least the following information:

- the identity and designated metric size of the tubing;
- whether the tubing was of regular-walled, thin-walled, extra-thin walled or ultra-thin walled type;
- whether the tubing shows visible breakage during the test;
- the date of testing;
- the type of stainless steel alloy used, chosen according to [Clause 4](#).

Table C.1 — Conditions for resistance to breakage test

Designated metric size	Distance between rigid support and point of application of bending force mm ±0,1
0,18	6
0,2	6
0,23	6
0,25	8
0,3	8
0,33	8
0,36	8
0,4	8
0,45	10
0,5	10
0,55	12,5
0,6	15
0,7	17,5
0,8	20
0,9	25
1,1	27,5
1,2	30
1,4	31,5
1,6	31,5
1,8	31,5
2,1	31,5
2,4	31,5
2,7	31,5
3	31,5
3,4	31,5

Annex D (normative)

Test method for resistance to corrosion

D.1 Principle

The tubing is partially immersed in sodium chloride solution for a specified time and afterwards the immersed portion compared visually with the unimmersed portion for signs of corrosion.

D.2 Reagents and apparatus

D.2.1 Solution of sodium chloride, $c(\text{NaCl}) = 0,5 \text{ mol/l}$ (analytical grade reagent) in distilled or deionized water of grade 3 in accordance with ISO 3696.

D.2.2 Selection of laboratory borosilicate glassware.

D.3 Procedure

Place a piece of needle tubing in a glass vessel ([D.2.2](#)) containing sodium chloride solution ([D.2.1](#)) at $(23 \pm 2) ^\circ\text{C}$, so that approximately half the length of the tubing is immersed. Maintain the liquid and tubing at $(23 \pm 2) ^\circ\text{C}$, for $7 \text{ h} \pm 5 \text{ min}$. Remove the needle tubing, wipe it dry and compare the immersed and un-immersed portions under normal or corrected vision for signs of corrosion caused by the immersion.

D.4 Test report

The test report shall contain at least the following information:

- the identity and designated metric size of the tubing;
- whether the tubing was of regular-walled, thin-walled, extra-thin walled or ultra-thin-walled type;
- whether corrosion occurred on the immersed half during the test;
- the date of testing;
- the type of stainless steel alloy used, chosen according to [Clause 4](#).

Annex E (informative)

Rationale with respect to test method for stiffness of tubing

E.1 General

This Annex provides rationale for the requirements of the stiffness test of [Table 2](#). This summary is intended for those who are familiar with the stiffness test indicated in this International Standard but who have not participated in its revision. An understanding of the approach and reasoning supporting the prescribed load conditions and maximum deflection limits is considered to be essential for proper application of the standard. Furthermore, as clinical practice and technology change, a documented rationale for the stiffness test will facilitate any revision of this International Standard necessitated by those developments.

The stiffness test requirements have been selected to strike a balance between objectives; namely that the test should be strict enough to ensure tubing of poor quality does not comply yet provide a reasonable expectation of compliance for tubing of acceptable quality. It was also the Committee's aim to avoid unnecessary and unintended burden on manufacturers that might occur as a result of fundamental changes in test methodology or hardware.

Therefore, the three-point-bending test configuration and the span prescribed for each designated metric size remain unchanged. The changes to the content of [Table 2](#) as compared with the prior revision of this International Standard have been limited to applied load at centre of the span and the respective acceptance criteria (maximum allowable deflection at the centre of the span).

Toward these stated objectives, the Committee took the following approach.

- a) Analyse the current loading conditions to establish reasonable bending moments to be applied for each tube (gage and wall thickness designation). While it should be considered acceptable to cause some amount of permanent deformation (i.e. yielding) during the test, the applied bending moment should not be greater than the expected maximum attainable (i.e. plastic moment). The moment applied should be selected based on expected ranges of
 - yield strength (between 205 MPa and 760 MPa),
 - Young's Modulus (between 150 GPa and 200 GPa apparent value based on experiment), and
 - plastic section modulus, Z (for each tube but limited by maximum and assumed least material conditions or "MMC" and LMC").
- b) Evaluate relationships between bending moment and deflection under limiting cases for assumed material behaviour
 - linear elastic (resulting in the lowest expected deflection), and
 - elastic-fully plastic (resulting in the greatest expected deflection).
- c) Specify the maximum allowable deflection for each tube designation considering the following:
 - fully annealed, LMC combinations should likely not be considered acceptable (i.e. should fail the test);
 - expectations of stiffness based on the previous revision of this International Standard;
 - empirical data and deviations from ideal behaviour.

Table E.1 — Definition of terms^{[4][5][6]}

Line	Term	Definition	Consistent units of measure for calculation
1	σ_y	Yield strength of the material	Pa
2	r_o, r_i	Outer radius and inner radius, respectively of the cross section	m
3	P	Applied load at the centre of the span	N
4	L	Width of span between supports	m
5	E	Young's modulus of the tube material	Pa
6	$I = \frac{\pi}{4} (r_o^4 - r_i^4)$	Area moment of inertia of the tube's cross section	m ⁴
7	$M = \frac{PL}{4}; M_y = \frac{P_y L}{4}; M_P = \frac{P_P L}{4}$	Bending moment at the centre of the span; Bending moment at the onset of yield; Fully plastic bending moment	Nm
8	$Z = \frac{M_P}{\sigma_y} = \frac{4}{3} (r_o^3 - r_i^3)$	Plastic section modulus for tubular cross section	m ³
9	$\delta = \frac{PL^3}{48EI} = \frac{PL^3}{12E\pi (r_o^4 - r_i^4)}$	Deflection at the beam centre (applicable within the linear elastic range of the material, i.e. prior to onset of yield)	m
10	$M_P = Z\sigma_y = \frac{4}{3} (r_o^3 - r_i^3) \sigma_y$	"Plastic moment" or value of the bending moment	Nm
11	$\sigma_{y,h}$	Yield strength of a strain hardened steel	Pa
12	$\sigma_{y,s}$	Yield strength of a fully annealed or soft steel	Pa

E.2 Determination of load

Implicit in the application of a three-point bend test with maximum allowable deflection is the expectation that the tubing sample should not collapse under the test conditions prescribed. Therefore, we begin with analysis of three-point bending of tubes of circular cross section to evaluate the material and geometric properties influencing bending strength and whether the load and span values specified in the previous edition of this International Standard are reasonable.

Subject to certain assumptions, the strength of a uniform cylindrical beam in three-point bending is determined by cross-sectional dimensions of the beam and the yield strength of its material. We may express the strength of a beam in terms of the maximum bending moment it may resist or "plastic

moment", M_p . For a load applied at the centre of the span and assuming elastic-perfectly plastic material behaviour, the plastic moment may be calculated as given in [Formula \(E.1\)](#)^[5]:

$$M_p = Z\sigma_y = \frac{4}{3}(r_o^3 - r_i^3)\sigma_y \quad (\text{E.1})$$

The value of "Z" or plastic section modulus is therefore a property only of inner and outer radii expressed as [Formula \(E.2\)](#):

$$Z = \frac{4}{3}(r_o^3 - r_i^3) \quad (\text{E.2})$$

The bending moment, M , applied to a beam in three-point bending may be expressed as a function of the span, L , and applied load, P , at the centre of the span as given in [Formula \(E.3\)](#):

$$M = \frac{PL}{4} \quad (\text{E.3})$$

Using these relationships and an assumed range of yield strength, we may compare the bending moments prescribed for the stiffness test to the plastic moments expected to cause failure for each tube. To achieve this, plastic section modulus Z is first tabulated for each tube at least material condition, or LMC, and maximum material condition, or MMC.

While MMC is easily defined using the greatest allowable outer diameter and the smallest allowable inner diameter for a specified tube, definition of the LMC requires an additional assumption. We should assume that the maximum allowable inner diameter for a given tube corresponds with the minimum allowable inner diameter for a tube of the same gauge but next thinner wall thickness designation.

NOTE Note that this approach is not intended to enforce a maximum inner diameter, but rather to establish bounds for analysis.

Thus, for example, the LMC condition is not defined for a TW tube if ISO does not define an ETW tube of the same gauge. In such cases, an alternate method is offered to estimate inner diameter for calculation of LMC plastic section modulus.

For cases of undefined LMC, the maximum allowable inner diameter is calculated by assuming proportionate moments of inertia. In this manner, we may determine a maximum inner diameter in these special cases. The example shown in [Formula \(E.4\)](#) to [Formula \(E.7\)](#) below illustrates the procedure to calculate the maximum inner diameter of a thin wall (TW) tube on the basis of the moments of inertia for the NW tube of the same designated metric size (i.e. gauge). An analogous approach is employed as needed for tubes of adjacent wall thickness designations (e.g. TW and ETW; ETW and UTW; or UTW).

$$\left[\frac{I_{\text{LMC}}}{I_{\text{MMC}}} \right]_{\text{NW}} = \left[\frac{I_{\text{LMC}}}{I_{\text{MMC}}} \right]_{\text{TW}} \quad (\text{E.4})$$

$$[I_{\text{LMC}}]_{\text{TW}} = \left[\frac{I_{\text{LMC}}}{I_{\text{MMC}}} \right]_{\text{NW}} [I_{\text{MMC}}]_{\text{TW}} \quad (\text{E.5})$$

$$\frac{\pi}{64} (D_{o,\text{MIN},\text{TW}}^4 - D_{i,\text{MAX},\text{TW}}^4) = [I_{\text{LMC}}]_{\text{TW}} = \left[\frac{I_{\text{LMC}}}{I_{\text{MMC}}} \right]_{\text{NW}} [I_{\text{MMC}}]_{\text{TW}} \quad (\text{E.6})$$

$$D_{i,\text{MAX},\text{TW}} = \left\{ D_{o,\text{MIN},\text{TW}}^4 - \frac{64}{\pi} \left[\frac{I_{\text{LMC}}}{I_{\text{MMC}}} \right]_{\text{NW}} [I_{\text{MMC}}]_{\text{TW}} \right\}^{1/4} \quad (\text{E.7})$$

The steel's yield strength influences both the point at which the relationship between load and deflection deviates from linear, as well as the maximum load the beam is expected to bear. Therefore, we should consider a range of yield strength over which to evaluate the relationship between load and

deflection in three-point bending. We estimate the yield strength of a 304 stainless steel^[4] between 205 MPa (fully annealed) and 760 MPa (half hard).

On the basis of the foregoing, we may estimate bending moment expected to induce failure, M_p , as a function of tubing dimensions and yield strength. Upper and lower bounds of M_p were obtained by evaluating M_p at the upper and lower bounds of material yield strength using [Formula \(E.8\)](#) and [Formula \(E.9\)](#):

$$M_{p,Hard} = Z\sigma_{y,Hard} = Z \times 760 \text{ MPa} \quad (\text{E.8})$$

$$M_{p,Soft} = Z\sigma_{y,Soft} = Z \times 205 \text{ MPa} \quad (\text{E.9})$$


By plotting the tabulated values (as per the previous edition of this International Standard) of bending moment M and plastic section modulus Z for both LMC and MMC conditions along with the relationships of [Formula \(E.8\)](#) and [Formula \(E.9\)](#), we have

M is the bending moment, in N-m;

Z is the plastic section modulus, in m^3 ;

$M_{p,H}$ is the plastic bending moment for yield strength of 760 MPa;

$M_{p,L}$ is the plastic bending moment for yield strength of 205 MPa.

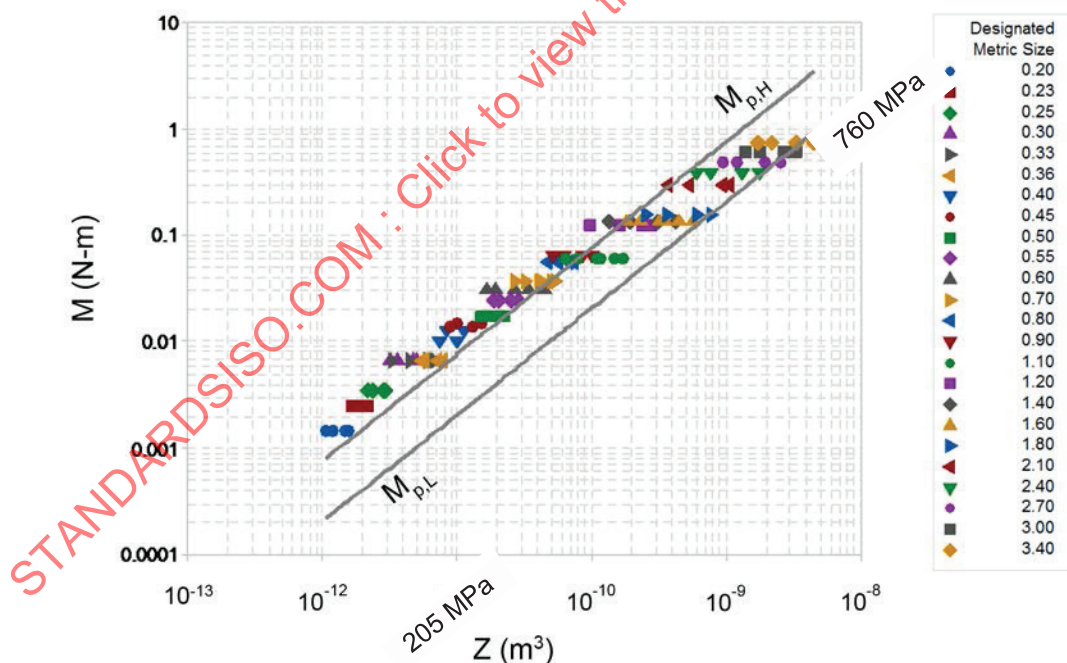

Key

M bending moment, in N-m

Z plastic section modulus, in m^3

$M_{p,H}$ plastic bending moment for yield strength of 760 MPa

$M_{p,L}$ plastic bending moment for yield strength of 205 MPa

Figure E.1 — ISO and fully plastic moment, M_p , versus plastic section modulus


We see by inspection of [Figure E.1](#) that many of the prescribed bending moments lie well above the predicted plastic moments even for material of 760 MPa yield strength in MMC; this International Standard is likely too stringent in many cases.

A reduction in prescribed bending moment for tubes between 1,4 mm and 0,20 mm designated metric size has been implemented. By “shifting” (i.e. prescribing a lower value) bending moment to become equal to the plastic moment corresponding to the lowest defined plastic section modulus of each gauge to the 760 MPa curve and specifying the same bending moment for each tube within the gauge, we have determined the proposed bending moments.

NOTE 1 Lowest defined section modulus is calculated using the smallest outer diameter for the designated metric size and the minimum inner diameter of the next thinner wall designation of the same designated metric size.

NOTE 2 Plastic section modulus is calculated on the basis of the newly defined dimensions for this revision of the International Standard; tubes that have changed since the 2001 version are ETW and UTW for 0,33 mm to 0,23 mm metric sizes; ETW for 0,2 mm metric size; and all 0,18 mm metric sizes.

This “shift” was only done for tubes where the plastic moment, M_p , for the lowest defined plastic section modulus is above the 760 MPa line. Then by substitution into [Formula \(E.3\)](#) and since span L has been maintained, the load P to be applied to each tube for stiffness testing was calculated.

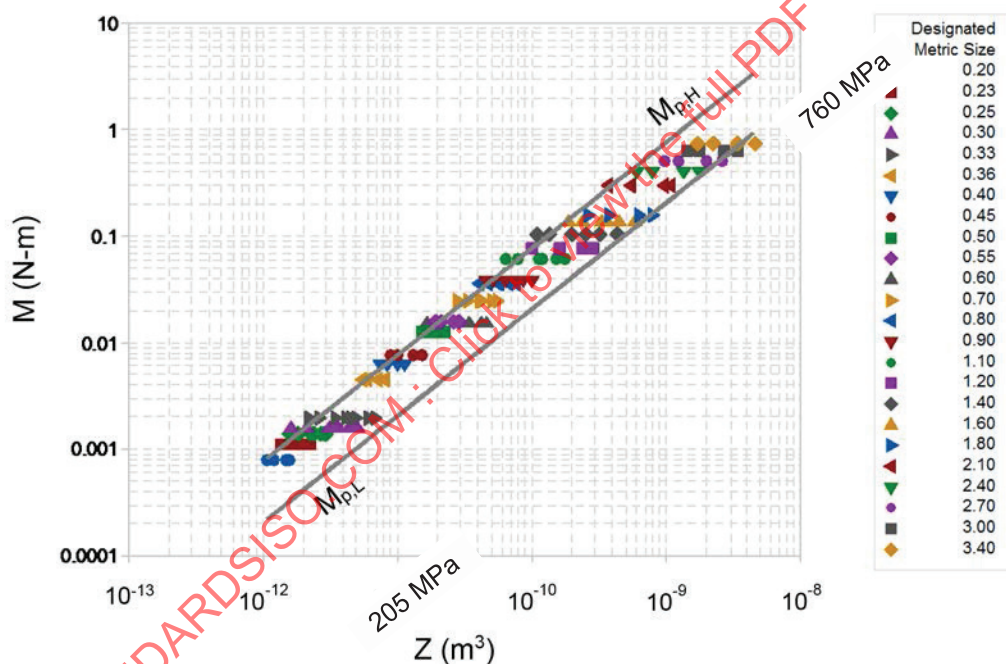

Key

M bending moment, in N-m

Z plastic section modulus, in m³

$M_{p,H}$ plastic bending moment for yield strength of 760 MPa

$M_{p,L}$ plastic bending moment for yield strength of 205 MPa

Figure E.2 — New bending moments for use in this International Standard and M_p versus plastic section modulus