



INTERNATIONAL ORGANIZATION FOR STANDARDIZATION

ISO RECOMMENDATION

R 695

DETERMINATION OF THE RESISTANCE OF GLASS TO ATTACK
BY A BOILING AQUEOUS SOLUTION OF MIXED ALKALI

1st EDITION
March 1968

COPYRIGHT RESERVED

The copyright of ISO Recommendations and ISO Standards belongs to ISO Member Bodies. Reproduction of these documents, in any country, may be authorized therefore only by the national standards organization of that country, being a member of ISO.

For each individual country the only valid standard is the national standard of that country.

Printed in Switzerland

Also issued in French and Russian. Copies to be obtained through the national standards organizations.

STANDARDSISO.COM : Click to view the full PDF of ISO/R 695:1968

BRIEF HISTORY

The ISO Recommendation R 695, *Determination of the resistance of glass to attack by a boiling aqueous solution of mixed alkali*, was drawn up by Technical Committee ISO/TC 48, *Laboratory glassware and related apparatus*, the Secretariat of which is held by the British Standards Institute (BSI).

Work on this question by the Technical Committee began in 1950 and led, in 1961, to the adoption of a Draft ISO Recommendation.

In December 1963, this Draft ISO Recommendation (No. 717) was circulated to all the ISO Member Bodies for enquiry. It was approved, subject to a few modifications of an editorial nature, by the following Member Bodies :

Argentina	France	New Zealand
Australia	Germany	Poland
Austria	Greece	Spain
Belgium	Hungary	Sweden
Brazil	India	Switzerland
Bulgaria	Israel	Turkey
Canada	Italy	U.A.R.
Chile	Japan	United Kingdom
Colombia	Korea, Rep. of	U.S.S.R.
Czechoslovakia	Netherlands	Yugoslavia

One Member Body opposed to the approval of the Draft :

U.S.A.

The Draft ISO Recommendation was then submitted by correspondence to the ISO Council, which decided, in March 1968, to accept it as an ISO RECOMMENDATION.

STANDARDSISO.COM : Click to view the full PDF of ISO/R 695:1968

DETERMINATION OF THE RESISTANCE OF GLASS TO ATTACK BY A BOILING AQUEOUS SOLUTION OF MIXED ALKALI

1. SCOPE

The purpose of this ISO Recommendation is to describe a method for determining the resistance of glass to attack by a boiling aqueous solution of equal volumes of *N* sodium carbonate and *N* sodium hydroxide. The resistance is measured inversely by the loss in mass per unit area of the glass.

2. APPARATUS

- 2.1 *Test vessel*, of pure silver or alkali-resistant silver alloy. A recommended vessel, as shown in the Figure overleaf, is cylindrical with a hemispherical base and has a close fitting lid. The lid has a wide neck and is fitted on the underside with four hooks from which to suspend the samples. Where a gasket is required to ensure an adequate joint between the body and the lid, it should be of a material which remains inert under the conditions of test.
- 2.2 *Condenser* of the Allihn or Liebig type, made of chemically resistant glass, fitted to the neck of the vessel through a bung of suitable inert material which has previously been boiled for 60 minutes in water.
- 2.3 *Balance accuracy* ± 0.1 mg.
- 2.4 *Desiccator*, containing a suitable drying agent.
- 2.5 *Measuring instruments*, suitable for measuring lengths and diameters to the required accuracy.
- 2.6 *Drying oven*, suitable for operation at a temperature of 150 °C.
- 2.7 *Beaker*, 1 litre capacity.
- 2.8 *Silver wire*.
- 2.9 *Tongs* tipped, if necessary, with a suitable material.

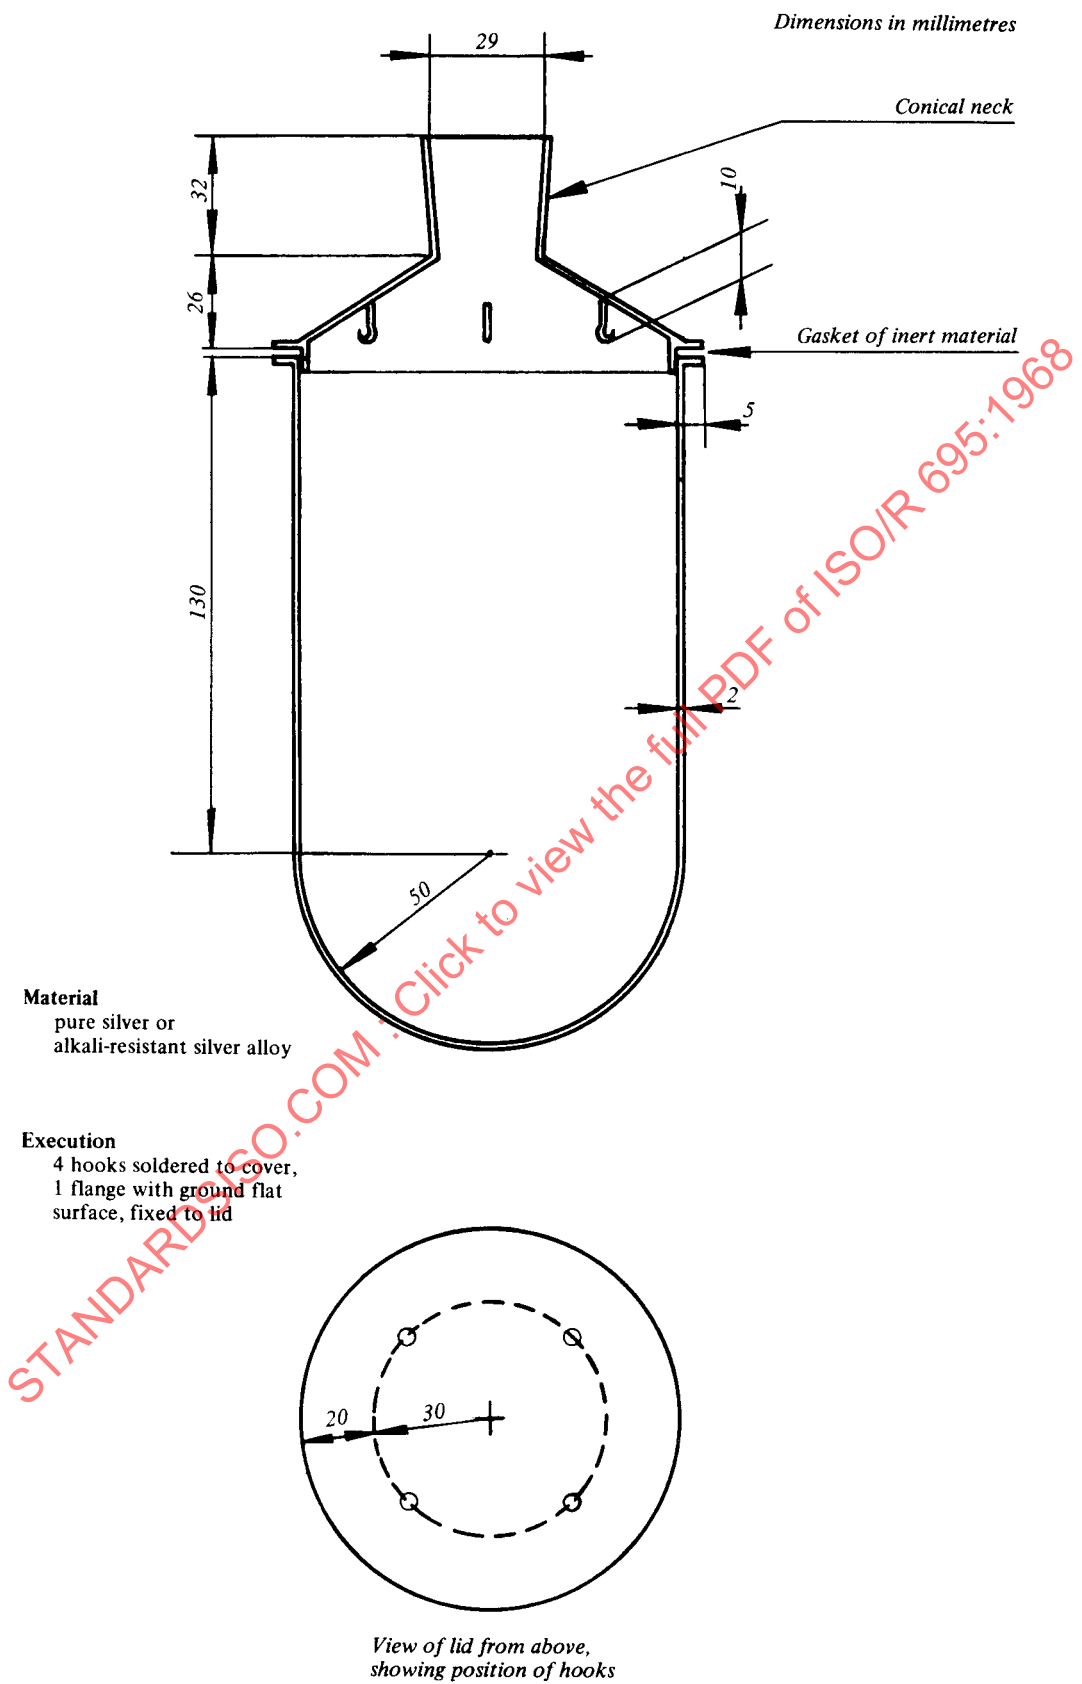


FIGURE – Example of suitable cylindrical silver vessel