
**Milk and milk products — Determination
of hen's egg white lysozyme by HPLC**

*Lait et produits laitiers — Détermination de lysozyme de blanc d'œufs
par CLHP*

STANDARDSISO.COM : Click to view the full PDF of ISO/TS 27105:2009



Reference numbers
ISO/TS 27105:2009(E)
IDF/RM 216:2009(E)

PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. Neither the ISO Central Secretariat nor the IDF accepts any liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies and IDF national committees. In the unlikely event that a problem relating to it is found, please inform the ISO Central Secretariat at the address given below.

STANDARDSISO.COM : Click to view the full PDF of ISO/TS 27105:2009



COPYRIGHT PROTECTED DOCUMENT

© ISO and IDF 2009

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO or IDF at the respective address below.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

International Dairy Federation
Diamant Building • Boulevard Auguste Reyers 80 • B-1030 Brussels
Tel. + 32 2 733 98 88
Fax + 32 2 733 04 13
E-mail info@fil-idf.org
Web www.fil-idf.org

Published in Switzerland

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

In other circumstances, particularly when there is an urgent market requirement for such documents, a technical committee may decide to publish other types of document:

- an ISO Publicly Available Specification (ISO/PAS) represents an agreement between technical experts in an ISO working group and is accepted for publication if it is approved by more than 50 % of the members of the parent committee casting a vote;
- an ISO Technical Specification (ISO/TS) represents an agreement between the members of a technical committee and is accepted for publication if it is approved by 2/3 of the members of the committee casting a vote.

An ISO/PAS or ISO/TS is reviewed after three years in order to decide whether it will be confirmed for a further three years, revised to become an International Standard, or withdrawn. If the ISO/PAS or ISO/TS is confirmed, it is reviewed again after a further three years, at which time it must either be transformed into an International Standard or be withdrawn.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO/TS 27105|IDF/RM 216 was prepared by Technical Committee ISO/TC 34, *Food products*, Subcommittee SC 5, *Milk and milk products*, and the International Dairy Federation (IDF). It is being published jointly by ISO and IDF.

Foreword

IDF (the International Dairy Federation) is a non-profit organization representing the dairy sector worldwide. IDF membership comprises National Committees in every member country as well as regional dairy associations having signed a formal agreement on cooperation with IDF. All members of IDF have the right to be represented on the IDF Standing Committees carrying out the technical work. IDF collaborates with ISO in the development of standard methods of analysis and sampling for milk and milk products.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the Action Teams and Standing Committees are circulated to the National Committees for voting. Publication as an International Standard requires approval by at least 50 % of the IDF National Committees casting a vote.

In other circumstances, particularly when there is an urgent market requirement for such documents, a Standing Committee may decide to publish an other type of normative document which is called by IDF: *Reviewed method*. Such a method represents an agreement between the members of a Standing Committee and is accepted for publication if it is approved by at least 50 % of the committee members casting a vote. A *Reviewed method* is equal to an ISO/PAS or ISO/TS and will, therefore, also be published jointly under ISO conditions.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. IDF shall not be held responsible for identifying any or all such patent rights.

ISO/TS 27105|IDF/RM 216 was prepared by the International Dairy Federation (IDF) and Technical Committee ISO/TC 34, *Food products*, Subcommittee SC 5, *Milk and milk products*. It is being published jointly by IDF and ISO.

All work was carried out by the Joint ISO-IDF Action Team on *Food additives and vitamins* of the Standing Committee on *Analytical methods for additives and contaminants* under the aegis of its project leaders, Dr. T. Berger (CH) and Prof. L. Pellegrino (IT).

Milk and milk products — Determination of hen's egg white lysozyme by HPLC

1 Scope

This Technical Specification specifies a method for the quantitative determination of hen's egg white lysozyme in milk and milk products.

The method is suitable for measuring low levels of hen's egg white lysozyme with a quantification limit of 5 mg/kg.

2 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

2.1

hen's egg white lysozyme content

mass fraction of substance determined by the procedure specified in this Technical Specification

NOTE The lysozyme content is expressed in milligrams per kilogram.

3 Principle

Casein and denatured whey proteins from milk and milk products are precipitated isoelectrically at pH 4,3 (cheese and solid milk products) or at pH 2,2 (milk and liquid milk products). Acid-soluble hen's egg white lysozyme is then determined by reversed-phase HPLC and fluorescence detection. The lysozyme peak can be verified by LC/MS (see annex A).

4 Reagents and reference substances

Use only reagents of recognized analytical grade, unless otherwise specified, and only distilled water or water of equivalent purity.

4.1 Reagents

4.1.1 Sodium chloride solution, $c(\text{NaCl}) = 1 \text{ mol/l}$.

Dissolve 58,44 g of sodium chloride in 1 l water.

4.1.2 Hydrochloric acid solution, $c(\text{HCl}) = 1 \text{ mol/l}$.

Add 4,0 ml of hydrochloric acid with mass fraction 37 % to a 50 ml one-mark volumetric flask (5.9). Make up to the mark with water and mix.

4.1.3 Sodium hydroxide solution, $c(\text{NaOH}) = 1 \text{ mol/l}$.

Add 2,6 ml of sodium hydroxide with a mass fraction of 50 % to a 50 ml one-mark volumetric flask (5.9). Make up to the mark with water and mix.

4.1.4 Trifluoroacetic acid (CF_3COOH).

4.1.5 Acetonitrile (CH_3CN), HPLC grade.

4.1.6 Water, HPLC grade.

4.2 Lysozyme

Pure hen's egg white lysozyme¹⁾.

NOTE Lysozyme (EC 3.2.1.17, muramidase) is an enzyme widely dispersed in nature, e.g. in hen's egg white (approximately 3 g/100 g to 4 g/100 g), saliva, and tear liquid. Lysozyme has a preservative effect because of the lytic activity on the cell wall of some bacteria. Hen's egg white lysozyme is used in cheesemaking to prevent late blowing of semi-hard and hard cheeses.

5 Apparatus and materials

Usual laboratory equipment and, in particular, the following.

5.1 pH-meter.

5.2 Fluted filter, of diameter 150 mm²⁾.

5.3 Membrane filter, of pore size 0,22 µm³⁾.

5.4 Balance, capable of weighing to the nearest 100 mg, with a readability of 10 mg.

5.5 Analytical balance, capable of weighing to the nearest 0,1 mg, with a readability of 0,01 mg.

5.6 Magnetic stirrer.

5.7 Homogenizer, capable of a rotational frequency of 2 500 r/min to 3 000 r/min.

5.8 HPLC equipment.

5.8.1 Elution gradient pumping system, capable of delivering a flow rate of 1,0 ml/min.

5.8.2 Manual or automatic injector, capable of injecting volumes of 50 µl.

5.8.3 Column heater, capable of maintaining a column temperature of 45 °C ± 2 °C.

1) Sigma L-7651 is an example of a suitable product available commercially. This information is given for the convenience of users of this Technical Specification and does not constitute an endorsement by ISO or IDF of this product.

2) Schleicher & Schuell 595½ is an example of a suitable product available commercially. This information is given for the convenience of users of this Technical Specification and does not constitute an endorsement by ISO or IDF of this product.

3) Millex-GV PVDF 0,22 µm is an example of a suitable product available commercially. This information is given for the convenience of users of this Technical Specification and does not constitute an endorsement by ISO or IDF of this product.

5.8.4 Column for reversed phase chromatography, PLRP-S 300 Å⁴⁾ 5 µm, 250 mm × 4,6 mm.

5.8.5 Fluorescence detector, capable of operating at 280 nm excitation and at 340 nm emission.

5.9 One-mark volumetric flasks, of capacities 10 ml and 50 ml, ISO 1042 ^[2] class A.

6 Sampling

A representative sample should have been sent to the laboratory. It should not have been damaged or changed during transport or storage.

Sampling is not part of the method specified in this Technical Specification. A recommended sampling method is given in ISO 707 | IDF 50^[1].

7 Procedure

7.1 Preparation of lysozyme standard solution

7.1.1 Lysozyme standard stock solution

Weigh, to the nearest 0,01 mg, 10 mg of lysozyme (4.2) into a 10 ml one-mark volumetric flask (5.9). Make up to the mark with sodium chloride solution (4.1.1) and mix.

Prepare the standard stock solutions on the day of use.

7.1.2 Lysozyme standard working solution

Pipette 80 µl of the lysozyme standard stock solution (7.1.1) into a 10 ml one-mark volumetric flask (5.9). Make up to the mark with sodium chloride solution (4.1.1) and mix.

The lysozyme standard working solution thus obtained contains 8,0 mg of lysozyme per litre.

7.2 Test portion

7.2.1 Milk or other liquid milk product

Weigh, to the nearest 0,01 g, 10,00 g of test sample into a 100 ml beaker.

7.2.2 Cheese or other solid milk products

Before weighing, grate the test samples of cheese. Weigh to the nearest 0,01 g, 2,00 g of test sample into a 100 ml beaker.

NOTE Soft cheese can be grated after freezing.

4) PLRP-S 300 Å is the trade name of a product supplied by Polymer Laboratories, Ltd. This information is given for the convenience of users of this document and does not constitute an endorsement by ISO or IDF of the product named. Equivalent products may be used if they can be shown to lead to the same results.

7.2.3 Preparation of test portion

Add 20 ml of sodium chloride solution (4.1.1) to the test portion (7.2.1 or 7.2.2) and mix. Adjust the pH of the solution obtained dropwise with sodium hydroxide solution (4.1.3) to pH 6,0.

Disperse the test portion for 30 s by using the homogenizer (5.7) at a frequency of 2 500 r/min to 3 000 r/min. Rinse the homogenizer in a separate 100 ml beaker using 10 ml of sodium chloride solution (4.1.1). Add the rinsings to the test solution.

Stir the beaker containing the test solution on a magnetic stirrer at room temperature for 1 h. Adjust the pH of the test portion obtained from milk and liquid milk products (7.2.1) to pH 2,2 and that obtained from cheese and solid milk products to pH 4,3 by using hydrochloric acid (4.1.2).

Transfer the test solution to a 50 ml one-mark volumetric flask (5.9). Use sodium chloride solution (4.1.1) to rinse the 100 ml beaker. Dilute to the mark with the sodium chloride solution (4.1.1) and mix.

Allow the test solution to stand at room temperature for 15 min.

Firstly, filter the test solution through a fluted filter (5.2) and then through the membrane filter (5.3) directly into a HPLC vial.

7.3 HPLC determination

7.3.1 Chromatographic conditions

Prepare the following:

- 1) stock solution I: 1 ml of trifluoroacetic acid (4.1.4) in 1 l of water (4.1.6).
- 2) stock solution II: 1 ml of trifluoroacetic acid (4.1.4) in 1 l of acetonitrile (4.1.5).

Use the following for HPLC:

- 1) elution solvent A containing: Stock solutions I and II with a mass fraction ratio I to II of 100:38,4.
- 2) elution solvent B containing: Stock solution II.

A suggested elution gradient is given in Table 1.

Table 1 — Suggested elution gradient

Time min	Elution solvent A ^a %	Elution solvent B ^a %
0,0	100	0
20,0	100	0
21,0	50	50
22,0	50	50
23,0	100	0
35,0	100	0
^a The elution gradient might require slight modification in order to achieve the resolution shown in Figure 1.		


Set the flow rate of the elution gradient pumping system of the HPLC equipment at 1,0 ml/min.

Set the temperature of the column heater at 45 °C. Determine the equilibration time by monitoring the column elution.

The detector response at the end of the run (baseline) should be equal to its initial value. An isocratic flushing of 15 min is usually sufficient.

Injection: Use a manual or automatic injector to inject 50 µl of the solutions (7.2.3) into the column.


HPLC fluorescence signals from the standard working solution (7.1.2) and a hard cheese sample (7.2.3) are given in Figures 1 and 2.

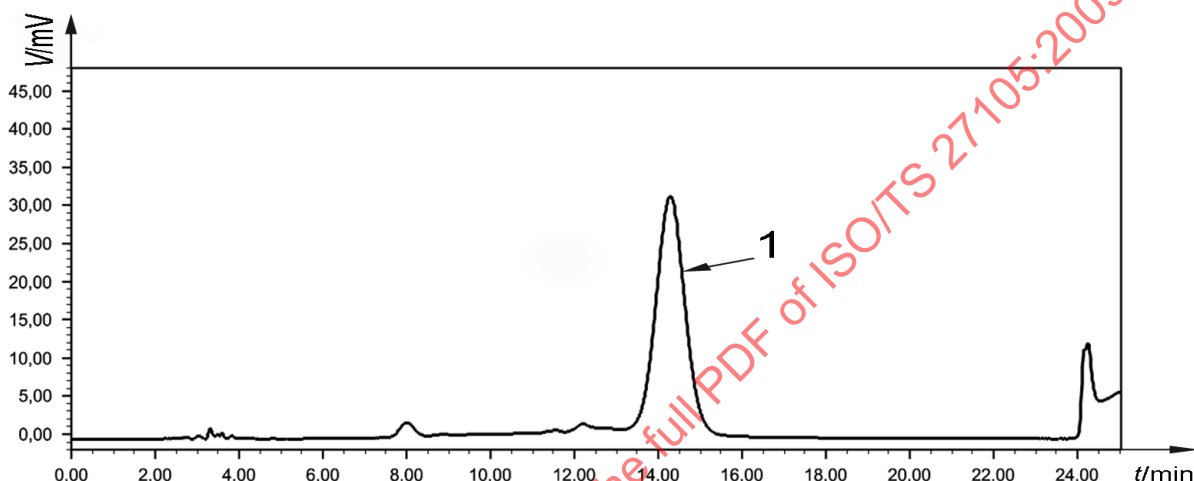

Key

- t time
- V peak response
- 1 lysozyme

Figure 1 — HPLC fluorescence signal from the standard working solution (7.1.2)

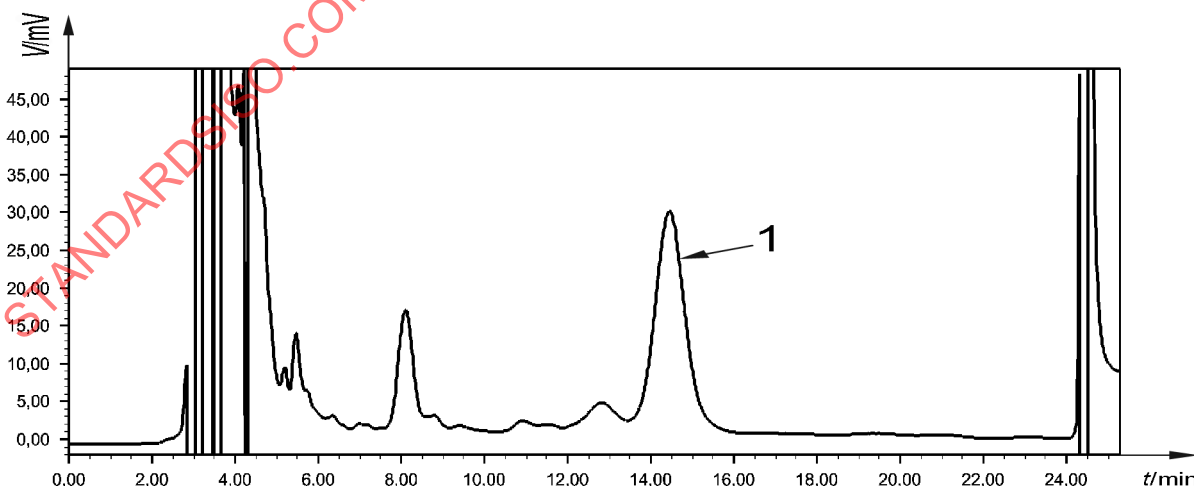

Key

- t time
- V peak response
- 1 lysozyme

Figure 2 — HPLC fluorescence signal from a hard cheese sample

8 Calculation and expression of results

8.1 Single-point calibration

Calculate the lysozyme content of the test sample, w_L , expressed in milligrams per kilogram, by using the following equation:

$$w_L = \frac{h_t \rho_s V_t}{h_s m_t}$$

where

ρ_s is the concentration, in milligrams per litre, of the standard working solution (7.1.2);

h_t is the numerical value of the peak height or area of the test solution (7.2), in counts;

h_s is the numerical value of the peak height or area of the standard working solution (7.1.2), in counts;

m_t is the mass, in grams, of the test portion (7.2);

V_t is the volume, in millilitres, of the test solution (7.2).

Check equipment linearity and reagent blank regularly.

8.2 Expression of results

Express the results to two decimal places. Express test results of below 5 mg/kg as: "less than 5 mg/kg".

9 Precision

This Technical Specification has not been tested and validated in an interlaboratory study. Precision values as well as detection limits are therefore not available.

Based on experience, the lowest limit of the lysozyme content quantification is 5 mg/kg (see 8.2).

10 Test report

The test report shall contain at least the following information:

- all information necessary for the complete identification of the sample;
- the sampling method used, if known;
- the test method used, with reference to this Technical Specification (ISO/TS 27105|IDF/RM 216:2009);
- all operational details not specified in this Technical Specification, or regarded as optional, together with details of any incident which may have influenced the test result(s);
- the test result(s) obtained, and, if the repeatability has been checked, the final quoted results obtained.

Annex A (informative)

Verification by LC/MS

A.1 General

For lysozyme peaks in the test solutions, findings can be verified using LC/MS. MS parameters for lysozyme have to be optimized and tuned according to the system manual of the instrument (e.g. needle voltage 3,0 kV, Probe 550 °C, cone voltage 130 V).

Use LC/MS equipment capable of running under the chromatographic conditions described in Clause A.3, which differ from those for HPLC (7.3) because trifluoroacetic acid is not used, and measure the mass signals $m/z = 1\,431$ $[M+H_{10}]^{10+}$; $1\,590$ $[M+H_9]^{9+}$ and $1\,788$ $[M+H_8]^{8+}$, retention time is approx. 12,5 min.

Verify the presence of lysozyme by homogeneous distribution of these masses all over the presumed lysozyme peak.

A.2 LC/MS equipment.

A.2.1 Elution gradient pumping system, capable of operating at 0,25 ml/min.

A.2.2 Manual or automatic injector, capable of injecting volumes of 5 µl.

A.2.3 Column heater, capable of being maintained at $40\text{ °C} \pm 2\text{ °C}$.

A.2.4 Column, reversed phase⁴⁾, 5 µm, 250 mm × 4,6 mm, conditioned for several hours without trifluoroacetic acid.

A.2.5 Mass spectrometer detector, capable of operating in ion mode ESI+ at m/z 1 431; 1 590; and 1 788.

A.3 Chromatographic conditions.

Use the following elution solvents for LC/MS:

- 1) elution solvent A containing 5 ml of formic acid (analytical grade) in 1 l of water (4.1.6).
- 2) elution solvent B containing 5 ml of formic acid in 1 l of acetonitrile (4.1.5).

Set the flow rate of the elution gradient pumping system of the HPLC equipment at 0,80 ml/min. The flow split should be: 0,5 ml/min MS; 0,3 ml/min waste (when 25 % B), motor valve 0,0 min eluent MS; 0,5 min eluent waste; 7,0 min eluent MS.

Using a manual or automatic injector, inject 5 µl.

A suggested elution gradient is given in Table A.1.